

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038545.D
 Acq On : 26 Jan 2023 12:33
 Operator : CG/JU
 Sample : PB150440BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK440

Quant Time: Jan 27 00:43:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1918	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	5126	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	3234	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	6629	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	5805	0.400	ng/ul	0.00
23) Perylene-d12	23.930	264	7434	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.338	96	12056	4.787	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1873	0.235	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	4507	0.272	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.729	202	834	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.769	252	1990	0.079	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038545.D
Acq On : 26 Jan 2023 12:33
Operator : CG/JU
Sample : PB150440BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK440

Quant Time: Jan 27 00:43:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

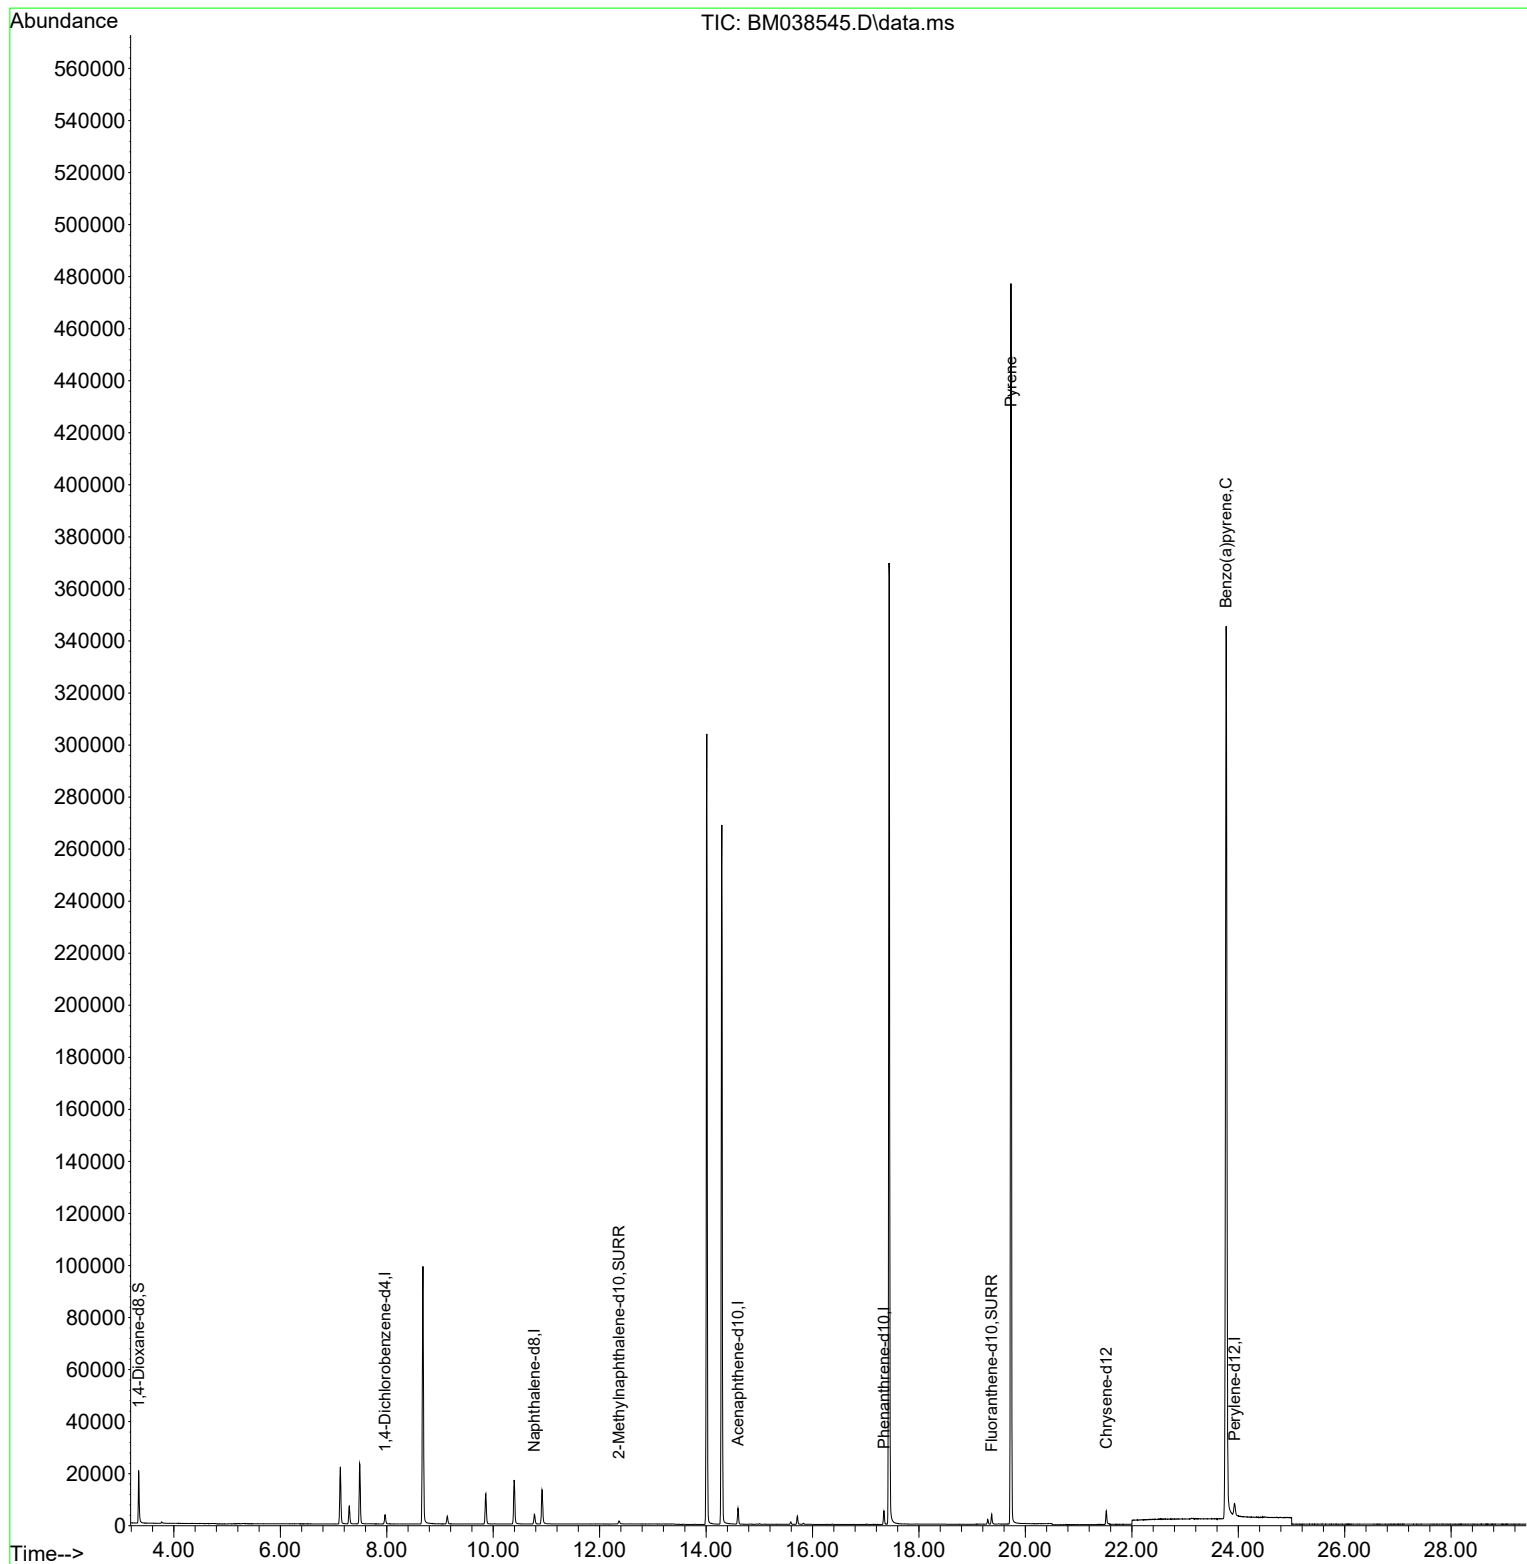

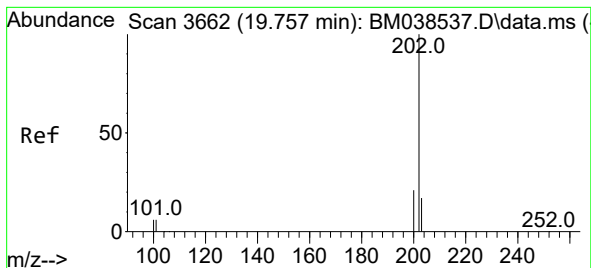

#20

Pyrene

Concen: 0.037 ng/ul

RT: 19.729 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM038545.D

Acq: 26 Jan 2023 12:33

Instrument :

BNA_M

ClientSampleId :

SBLK440





Tgt Ion:202 Resp: 834

Ion Ratio Lower Upper

202 100

101 139.0 5.9 8.9#

100 1022.6 5.2 7.8#

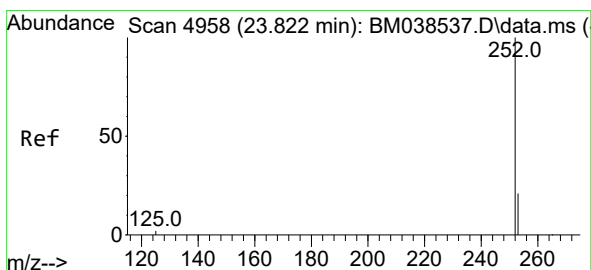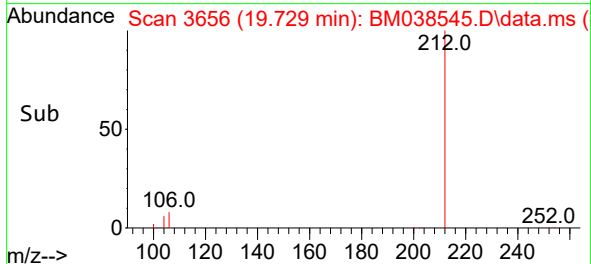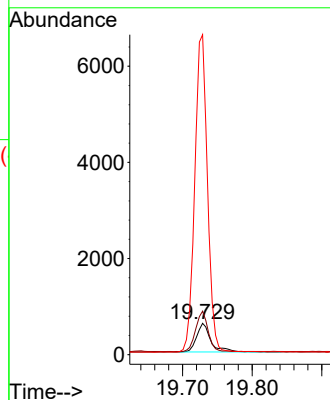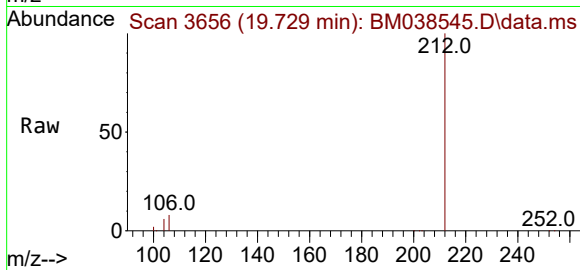

#26

Benzo(a)pyrene

Concen: 0.079 ng/ul

RT: 23.769 min Scan# 4940

Delta R.T. -0.053 min

Lab File: BM038545.D

Acq: 26 Jan 2023 12:33

Tgt Ion:252 Resp: 1990

Ion Ratio Lower Upper

252 100

253 62.3 25.1 37.7#

125 42.4 10.0 15.0#

