

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038554.D
 Acq On : 26 Jan 2023 18:49
 Operator : CG/JU
 Sample : PB150402BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK402

Quant Time: Jan 27 00:44:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1538	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	4088	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	2633	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	5244	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	5201	0.400	ng/ul	0.00
23) Perylene-d12	23.930	264	7604	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	8836	4.375	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1353	0.213	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	3307	0.223	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.729	202	667	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.769	252	1785	0.069	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038554.D
Acq On : 26 Jan 2023 18:49
Operator : CG/JU
Sample : PB150402BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK402

Quant Time: Jan 27 00:44:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

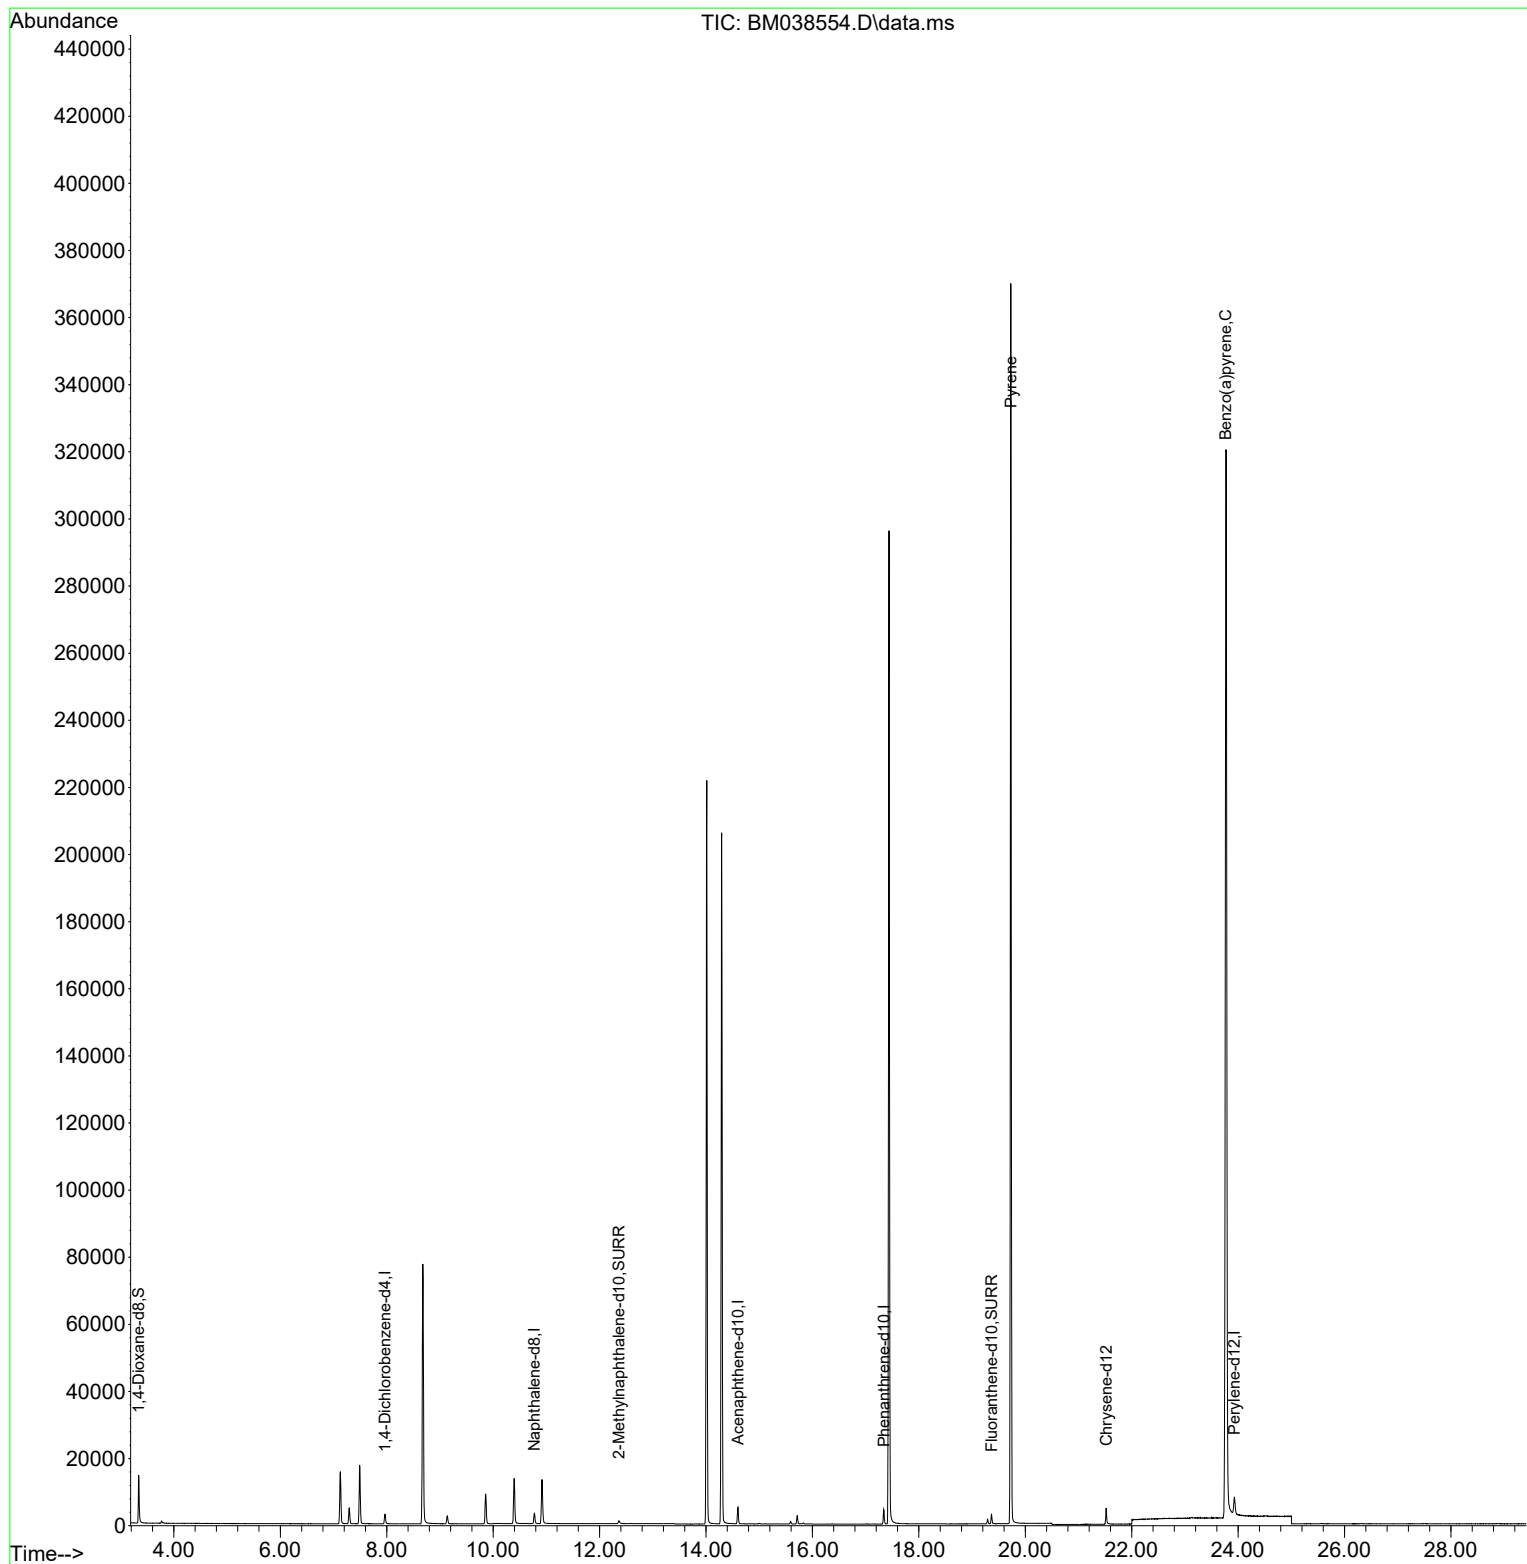

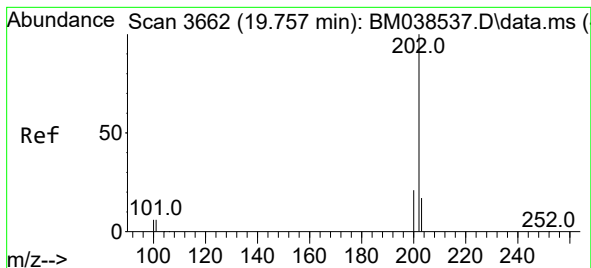

#20

Pyrene

Concen: 0.033 ng/ul

RT: 19.729 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM038554.D

Acq: 26 Jan 2023 18:49

Instrument :





BNA_M

ClientSampleId :

SBLK402

Tgt Ion:202 Resp: 667

Ion	Ratio	Lower	Upper
202	100		
101	151.7	5.9	8.9#
100	1117.3	5.2	7.8#

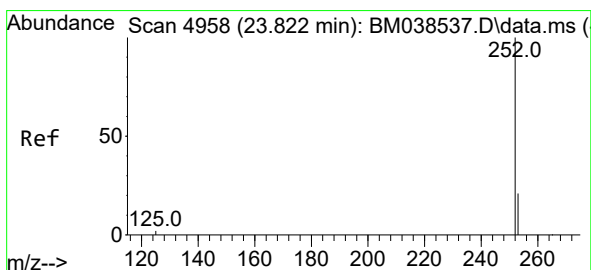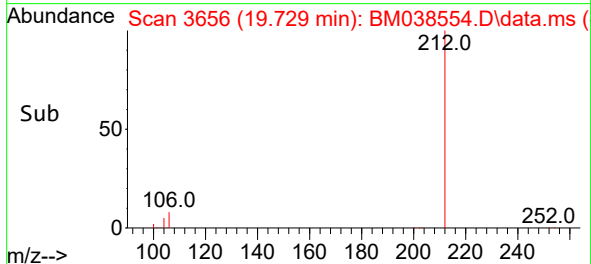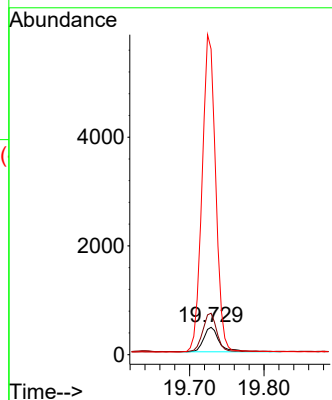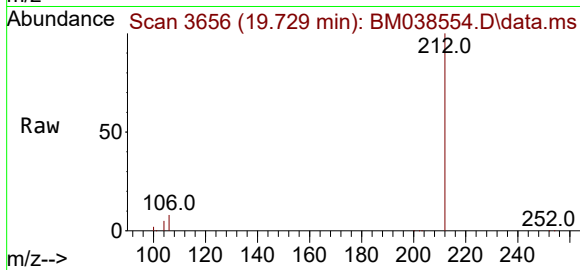

#26

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.769 min Scan# 4940

Delta R.T. -0.053 min

Lab File: BM038554.D

Acq: 26 Jan 2023 18:49

Tgt Ion:252 Resp: 1785

Ion	Ratio	Lower	Upper
252	100		
253	62.4	25.1	37.7#
125	39.2	10.0	15.0#

