

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038555.D
 Acq On : 26 Jan 2023 19:26
 Operator : CG/JU
 Sample : PB150403BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK403

Quant Time: Jan 27 00:44:43 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1358	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	3454	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	2258	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	4854	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	5304	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	7911	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.343	96	9153	5.133	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1355	0.253	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	3819	0.252	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.591	166	598	0.063	ng/ul#	20
20) Pyrene	19.729	202	750	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.766	252	2005	0.075	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038555.D
Acq On : 26 Jan 2023 19:26
Operator : CG/JU
Sample : PB150403BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK403

Quant Time: Jan 27 00:44:43 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration




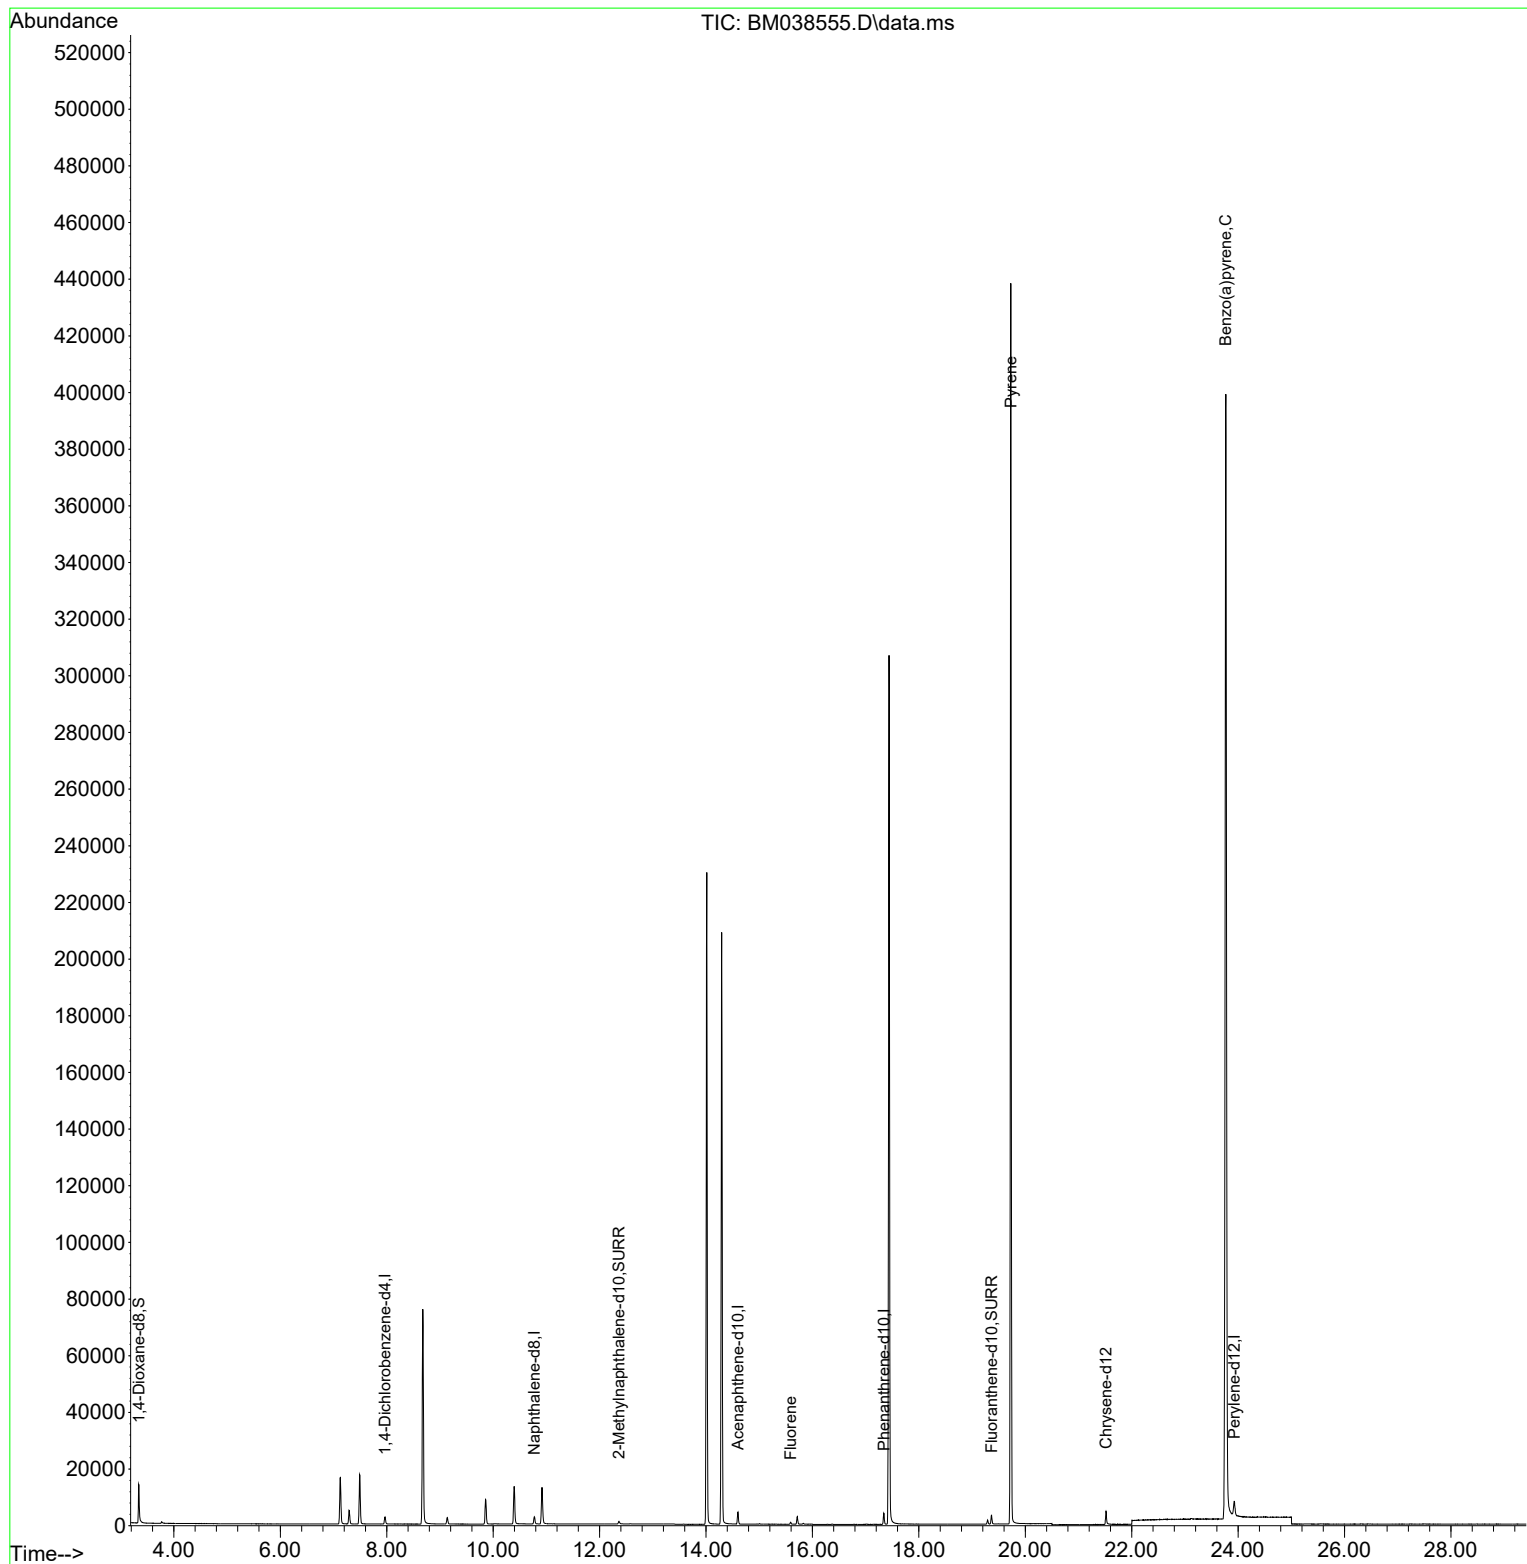


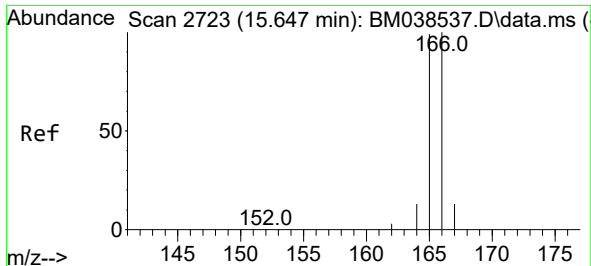

#12
Fluorene
Concen: 0.063 ng/ul
RT: 15.591 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM038555.D
Acq: 26 Jan 2023 19:26




Instrument :
BNA_M
ClientSampleId :
SBLK403


Tgt Ion:166 Resp: 598
Ion Ratio Lower Upper
166 100
165 16.3 79.3 118.9#
167 40.3 11.9 17.9#

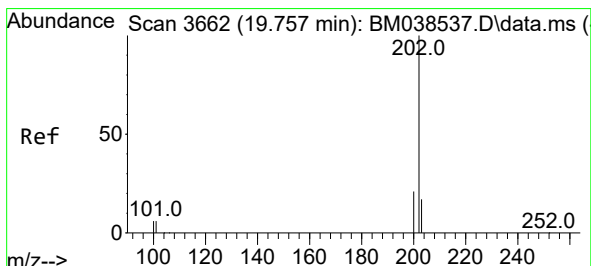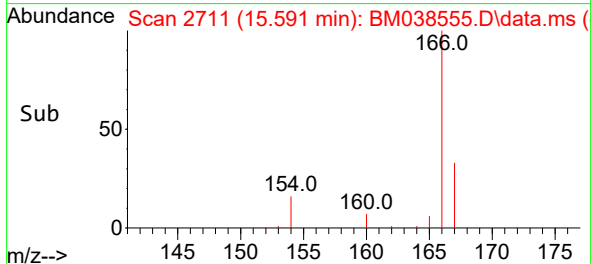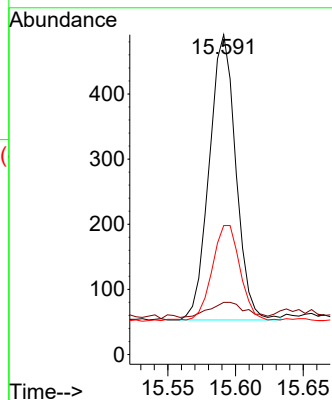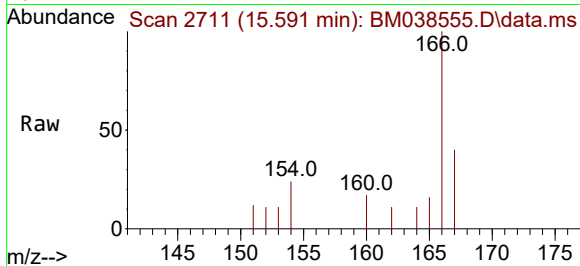

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.729 min Scan# 3656
Delta R.T. -0.028 min
Lab File: BM038555.D
Acq: 26 Jan 2023 19:26


Tgt Ion:202 Resp: 750
Ion Ratio Lower Upper
202 100
101 134.8 5.9 8.9#
100 1023.5 5.2 7.8#

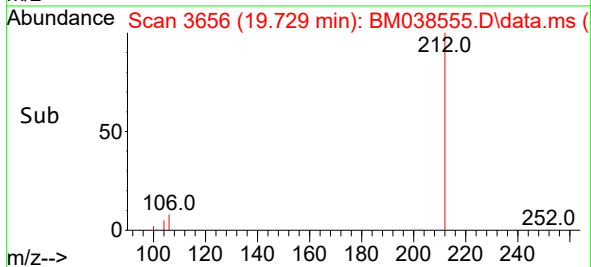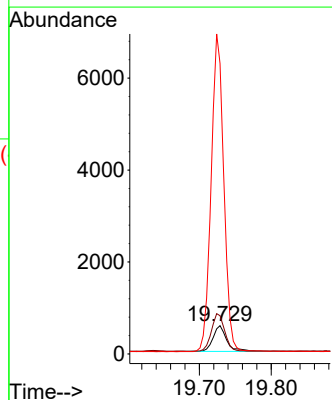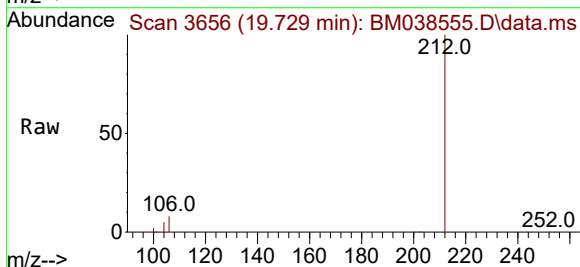

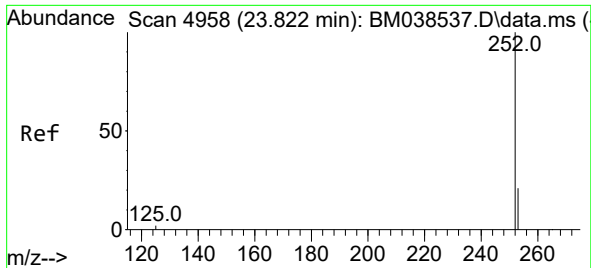

#26
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.766 min Scan# 4958
Delta R.T. -0.056 min
Lab File: BM038555.D
Acq: 26 Jan 2023 19:26

Instrument :
BNA_M
ClientSampleId :
SBLK403

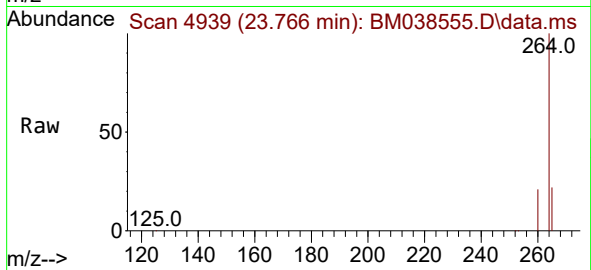

Tgt Ion:252 Resp: 2005
Ion Ratio Lower Upper
252 100
253 57.7 25.1 37.7#
125 34.4 10.0 15.0#

