

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038560.D
 Acq On : 26 Jan 2023 22:32
 Operator : CG/JU
 Sample : PB150406BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK406

Quant Time: Jan 27 00:45:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1394	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	3996	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	2716	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	5536	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	4754	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	6441	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	10160	5.550	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1725	0.278	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	4161	0.306	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.729	202	841	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.769	252	1877	0.086	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038560.D
Acq On : 26 Jan 2023 22:32
Operator : CG/JU
Sample : PB150406BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK406

Quant Time: Jan 27 00:45:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

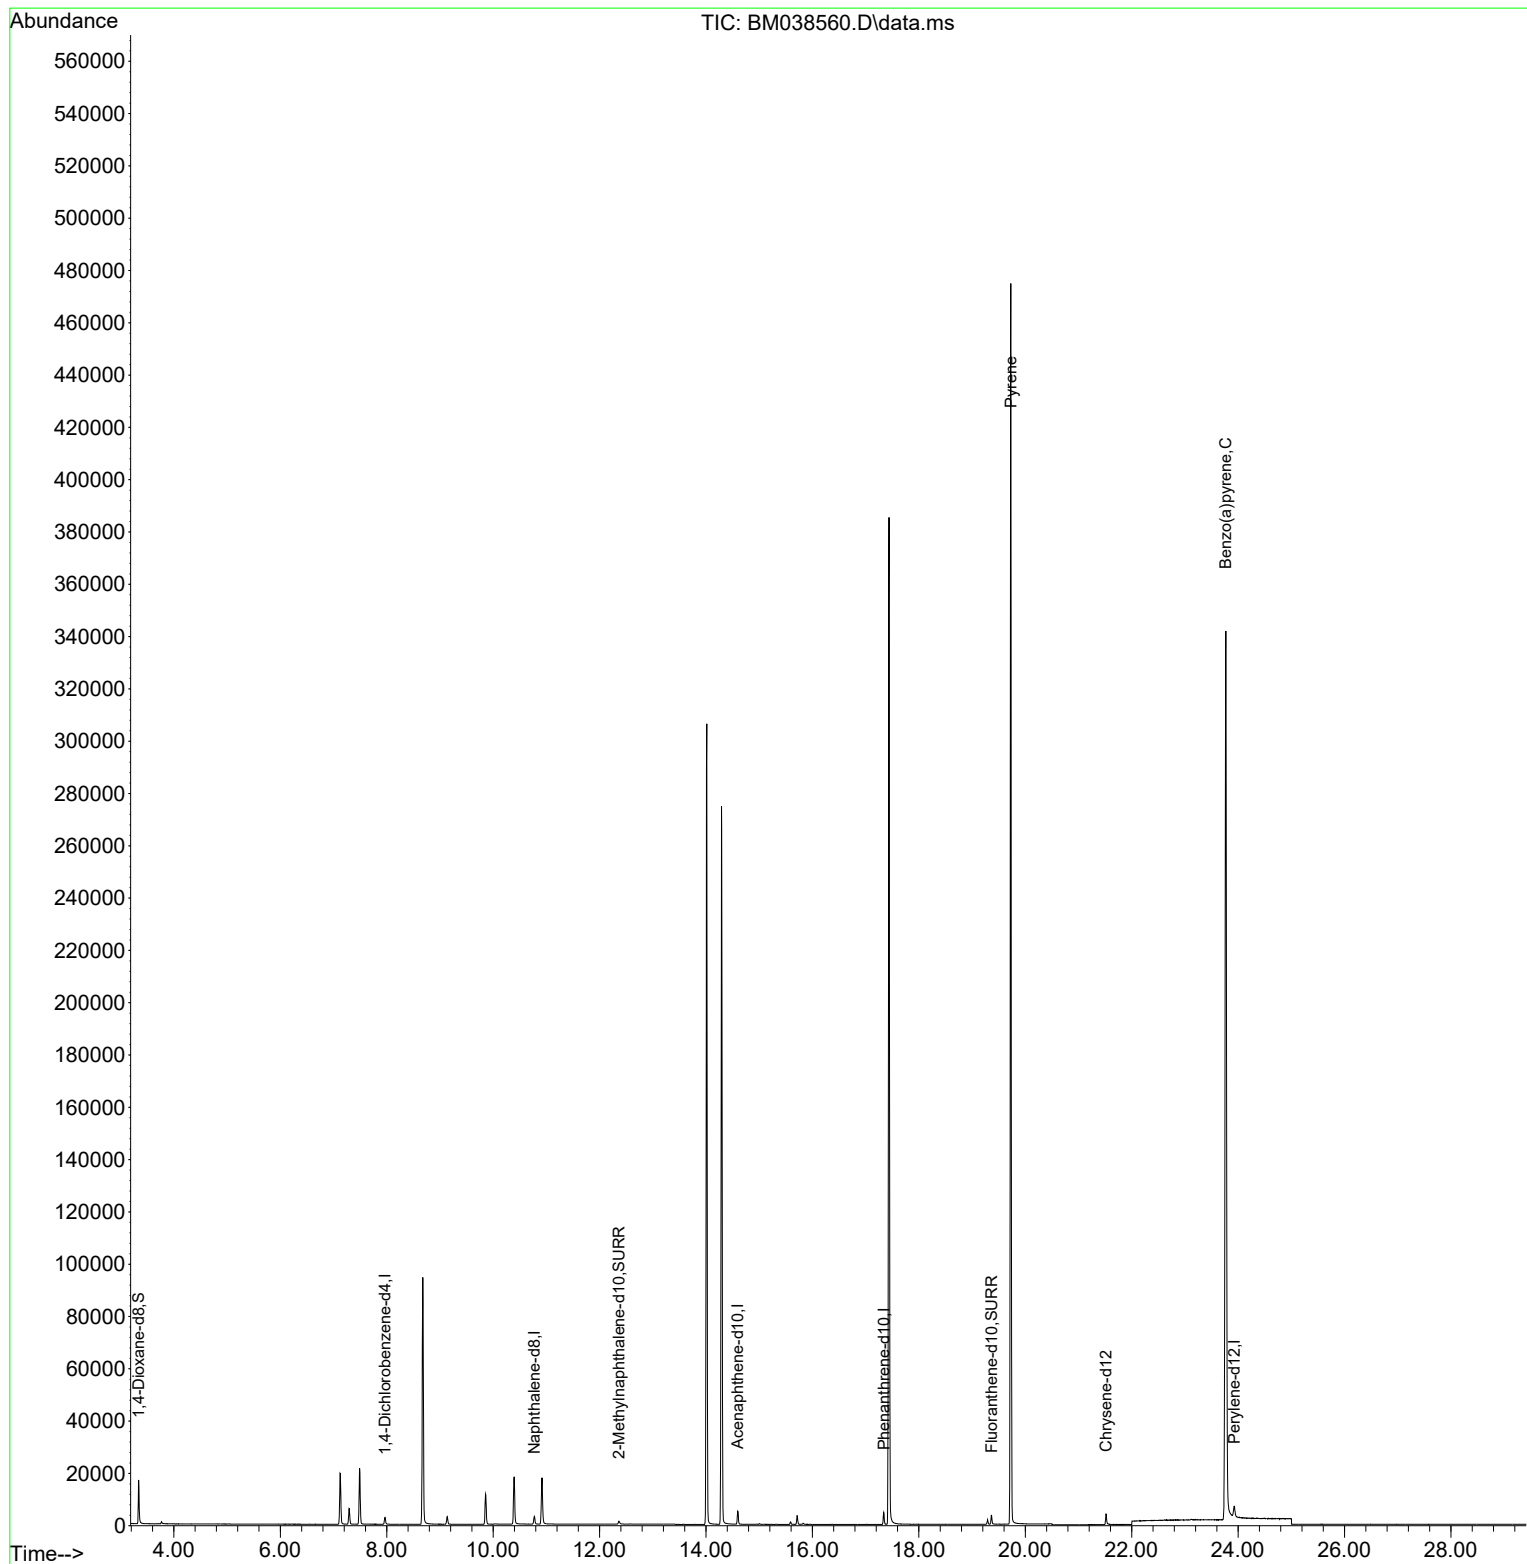

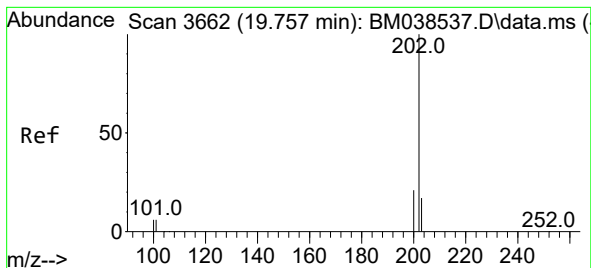

#20

Pyrene

Concen: 0.046 ng/ul

RT: 19.729 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM038560.D

Acq: 26 Jan 2023 22:32

Instrument :

BNA_M

ClientSampleId :

SBLK406





Tgt Ion:202 Resp: 841

Ion Ratio Lower Upper

202 100

101 138.1 5.9 8.9#

100 1051.3 5.2 7.8#

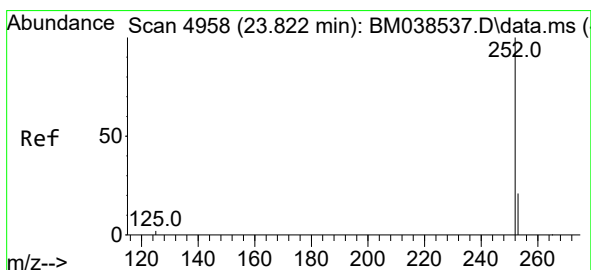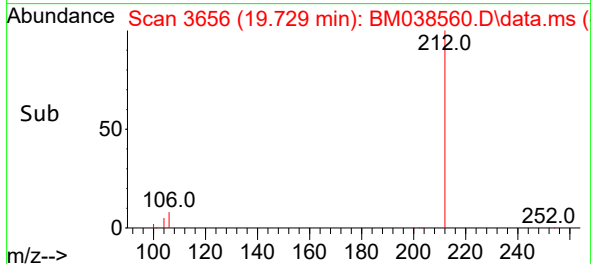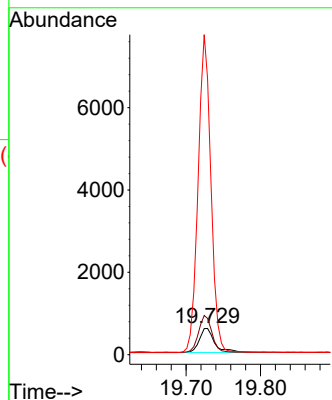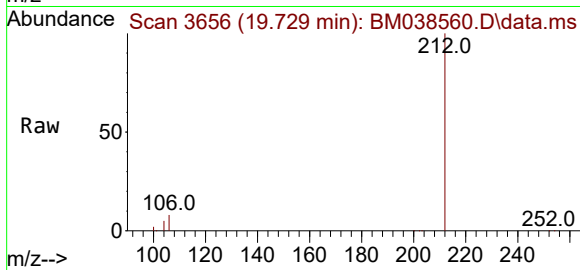

#26

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.769 min Scan# 4940

Delta R.T. -0.053 min

Lab File: BM038560.D

Acq: 26 Jan 2023 22:32

Tgt Ion:252 Resp: 1877

Ion Ratio Lower Upper

252 100

253 60.3 25.1 37.7#

125 38.0 10.0 15.0#

