

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038590.D
 Acq On : 27 Jan 2023 18:08
 Operator : CG/JU
 Sample : PB150412BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK412

Quant Time: Jan 27 22:00:45 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	1412	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	4218	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	2763	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	5877	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	4709	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	5938	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.338	96	9913	5.346	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1923	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	4405	0.328	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.587	166	763	0.066	ng/ul#	17
20) Pyrene	19.724	202	746	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.760	252	1557	0.078	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038590.D
Acq On : 27 Jan 2023 18:08
Operator : CG/JU
Sample : PB150412BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK412

Quant Time: Jan 27 22:00:45 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration




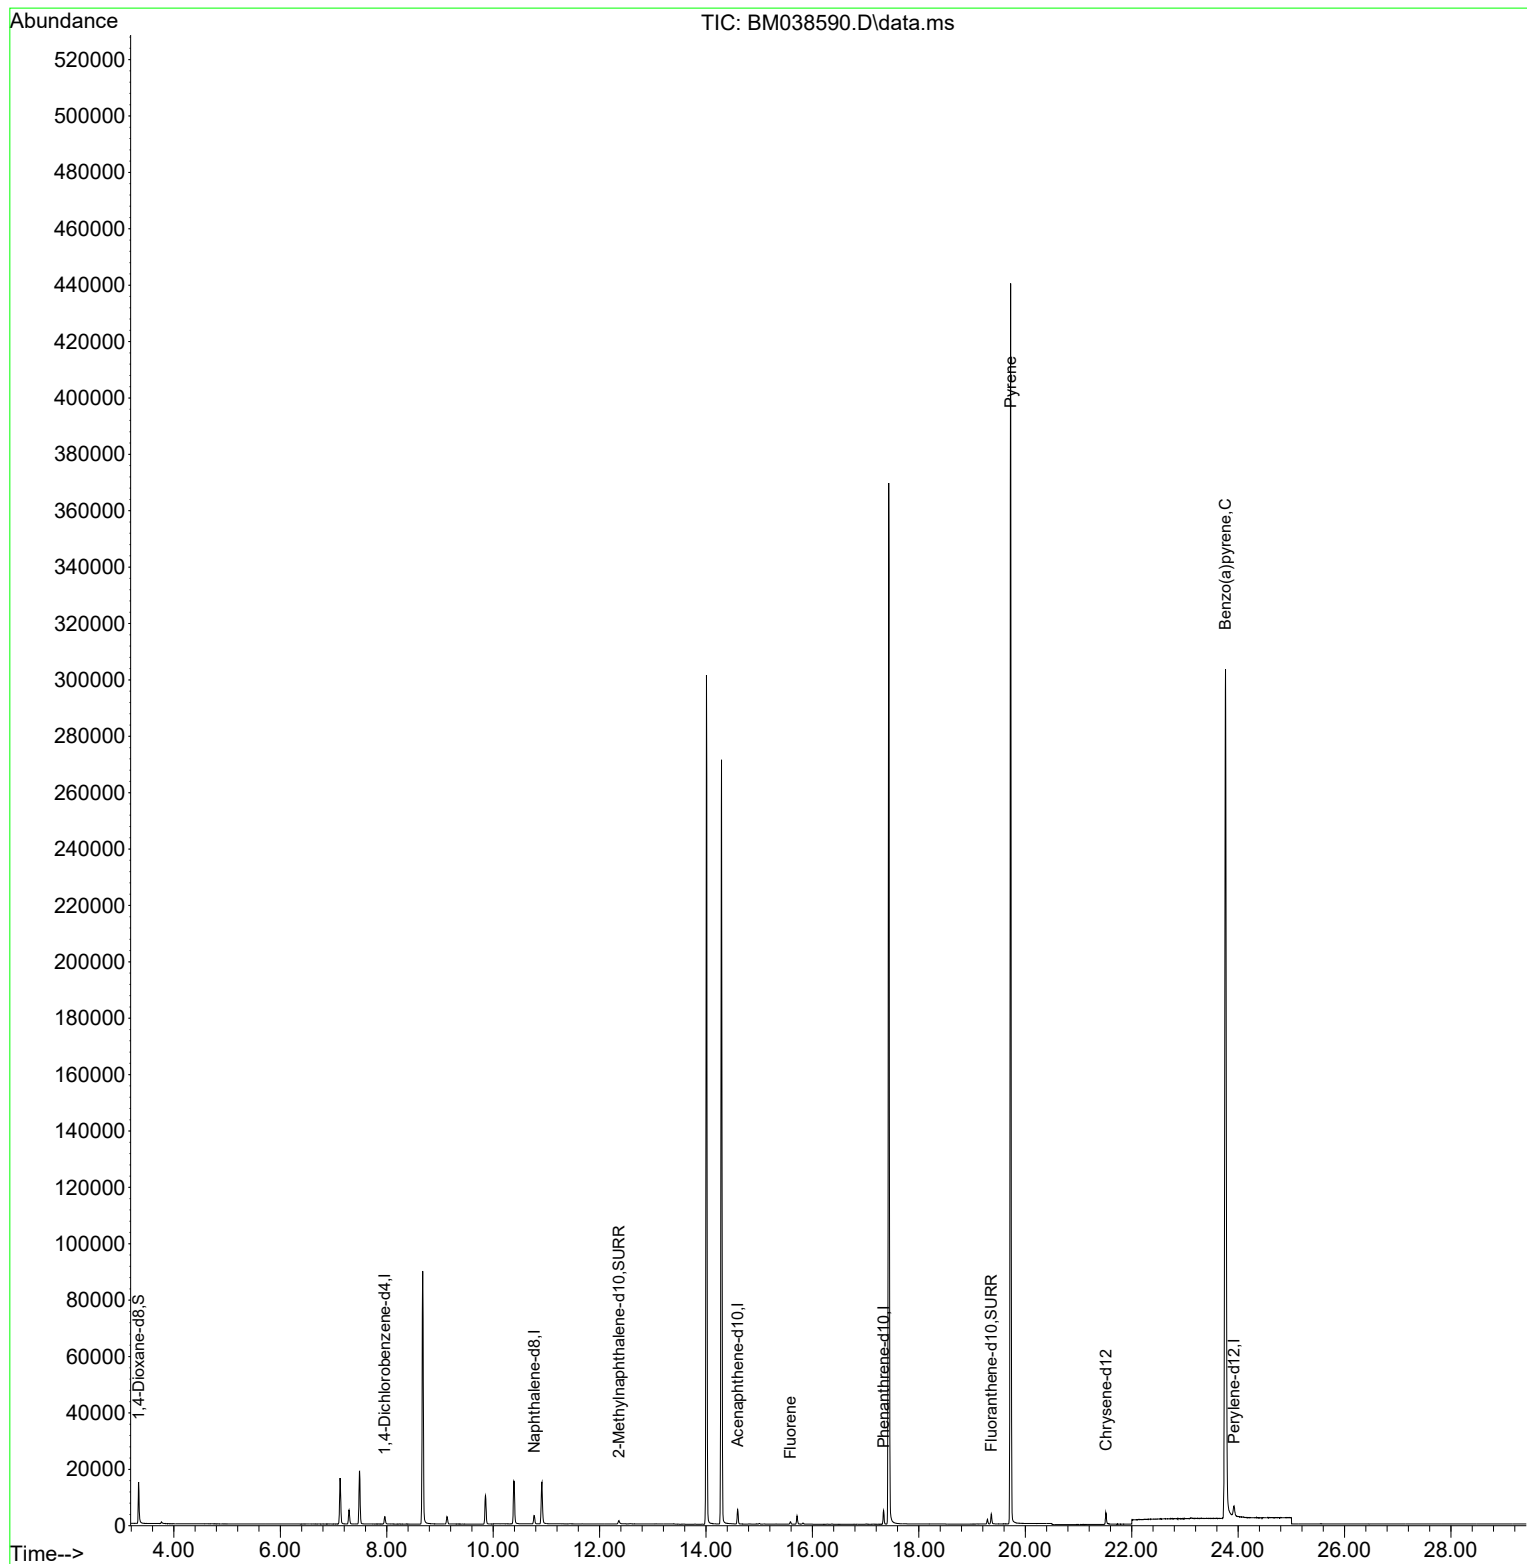


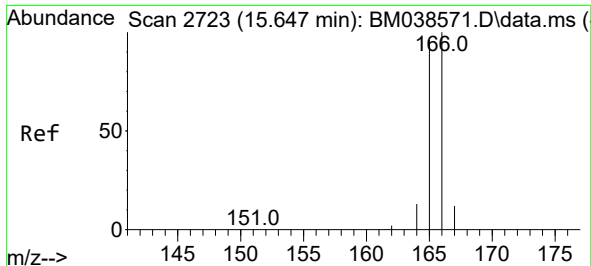

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.587 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM038590.D
Acq: 27 Jan 2023 18:08




Instrument :
BNA_M
ClientSampleId :
SBLK412


Tgt Ion:166 Resp: 763
Ion Ratio Lower Upper
166 100
165 14.0 79.3 118.9#
167 41.0 11.9 17.9#

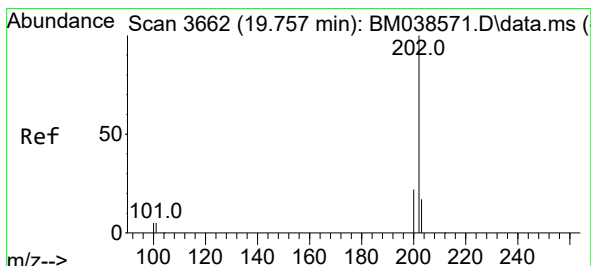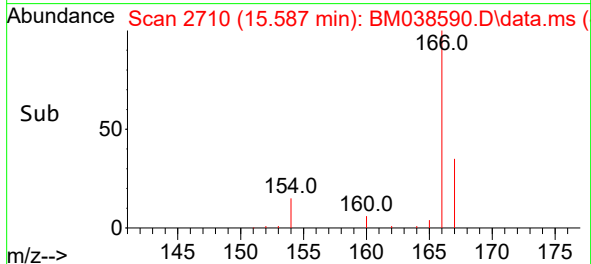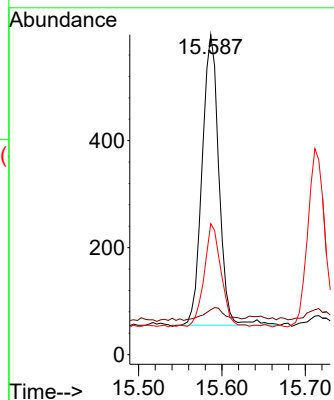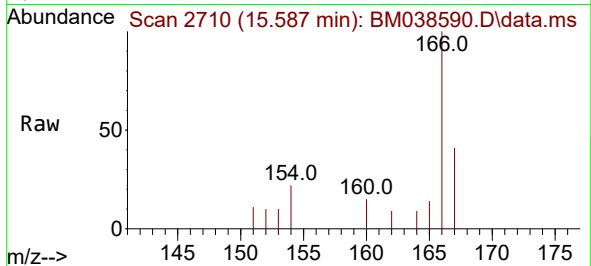

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.724 min Scan# 3655
Delta R.T. -0.033 min
Lab File: BM038590.D
Acq: 27 Jan 2023 18:08


Tgt Ion:202 Resp: 746
Ion Ratio Lower Upper
202 100
101 138.7 5.9 8.9#
100 1078.7 5.2 7.8#

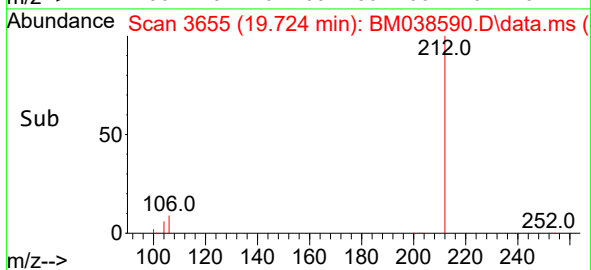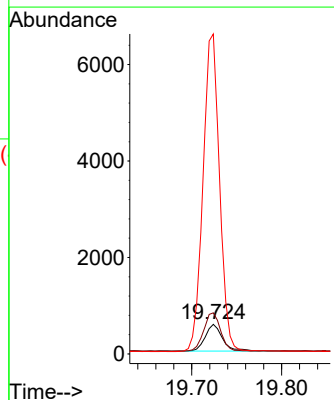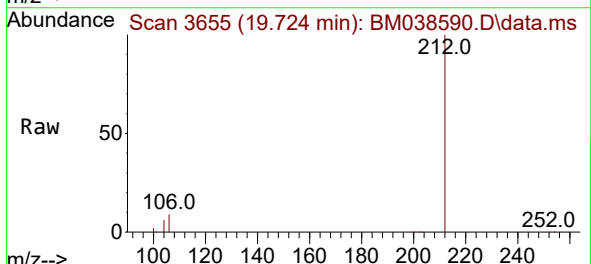

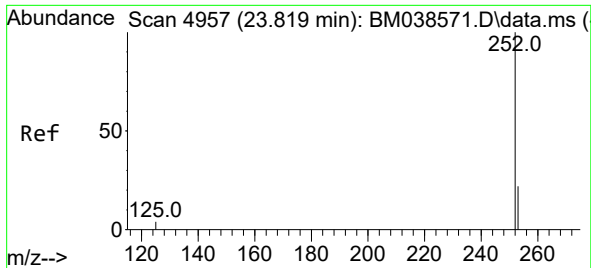

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.760 min Scan# 4957
Delta R.T. -0.062 min
Lab File: BM038590.D
Acq: 27 Jan 2023 18:08

Instrument :
BNA_M
ClientSampleId :
SBLK412

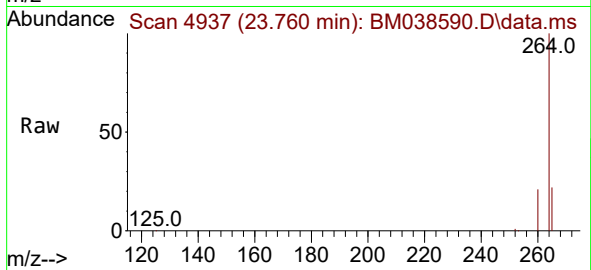

Tgt Ion:252 Resp: 1557
Ion Ratio Lower Upper
252 100
253 65.0 25.1 37.7#
125 37.8 10.0 15.0#

