




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038550.D
Acq On : 26 Jan 2023 15:40
Operator : CG/JU
Sample : 01226-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F8

Manual IntegrationsAPPROVED

Quant Time: Jan 27 00:44:06 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/27/2023
Supervised By :mohammad ahmed 01/30/2023

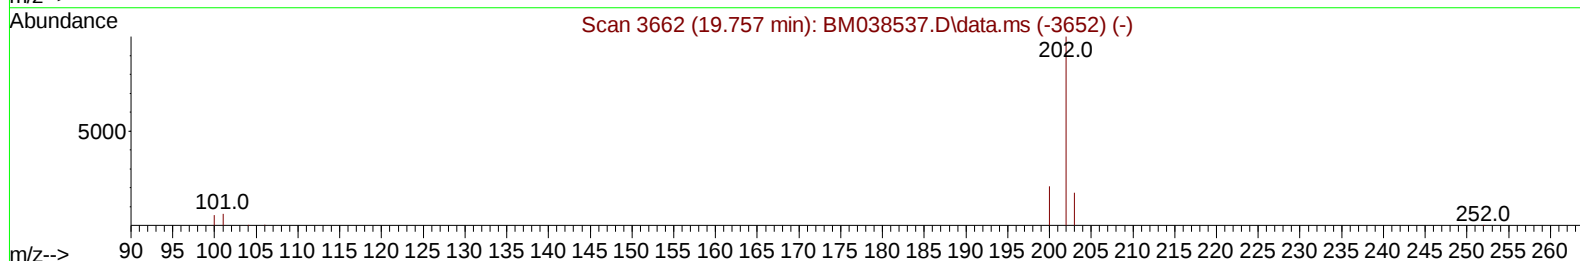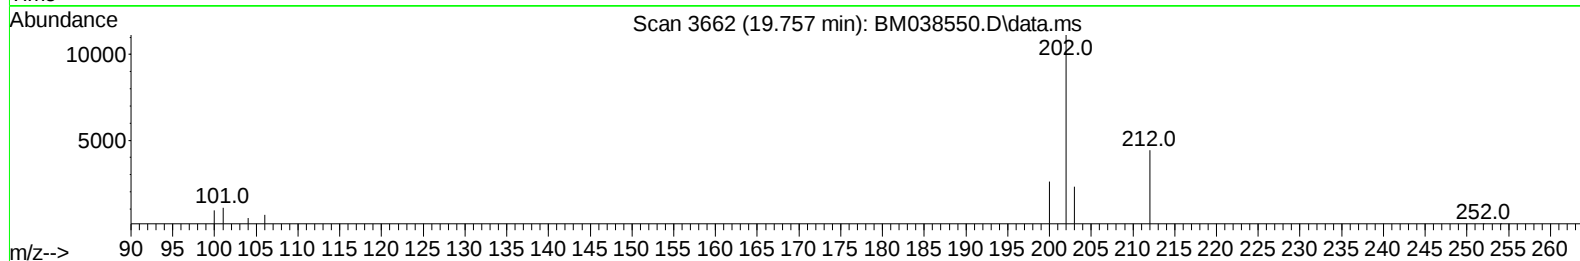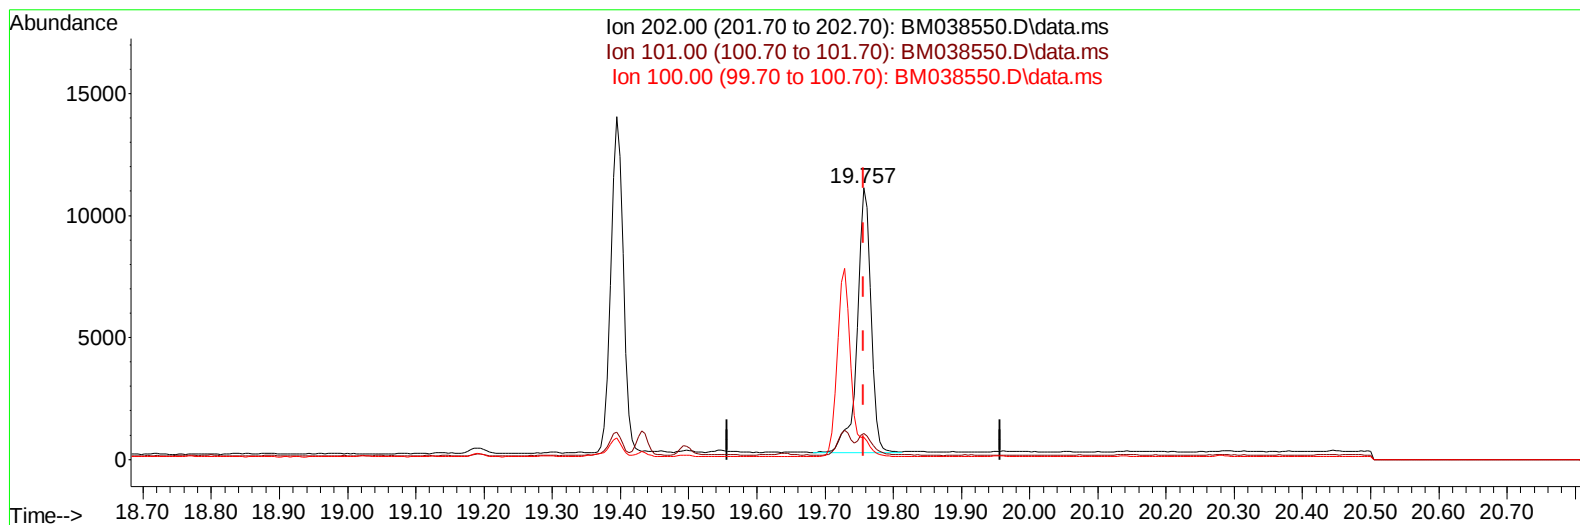

TIC: BM038550.D\data.ms

(20) Pyrene

19.757min (-0.000) 0.52 ng/u1

response 15131

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.40	9.56#
100.00	6.50	8.17#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038550.D
Acq On : 26 Jan 2023 15:40
Operator : CG/JU
Sample : 01226-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F8

Manual IntegrationsAPPROVED

Quant Time: Jan 27 00:44:06 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/27/2023
Supervised By :mohammad ahmed 01/30/2023

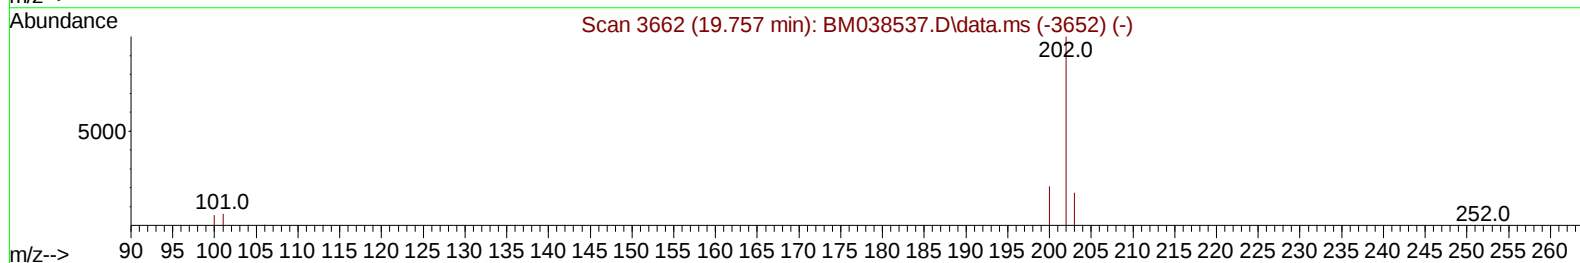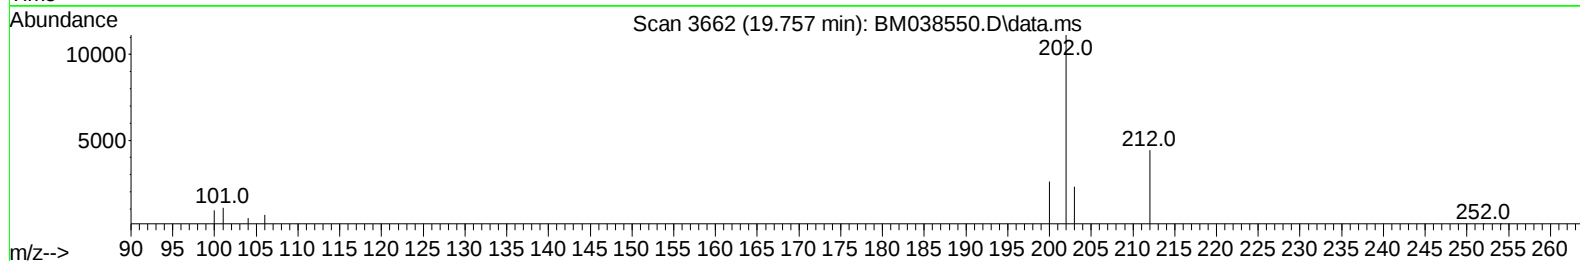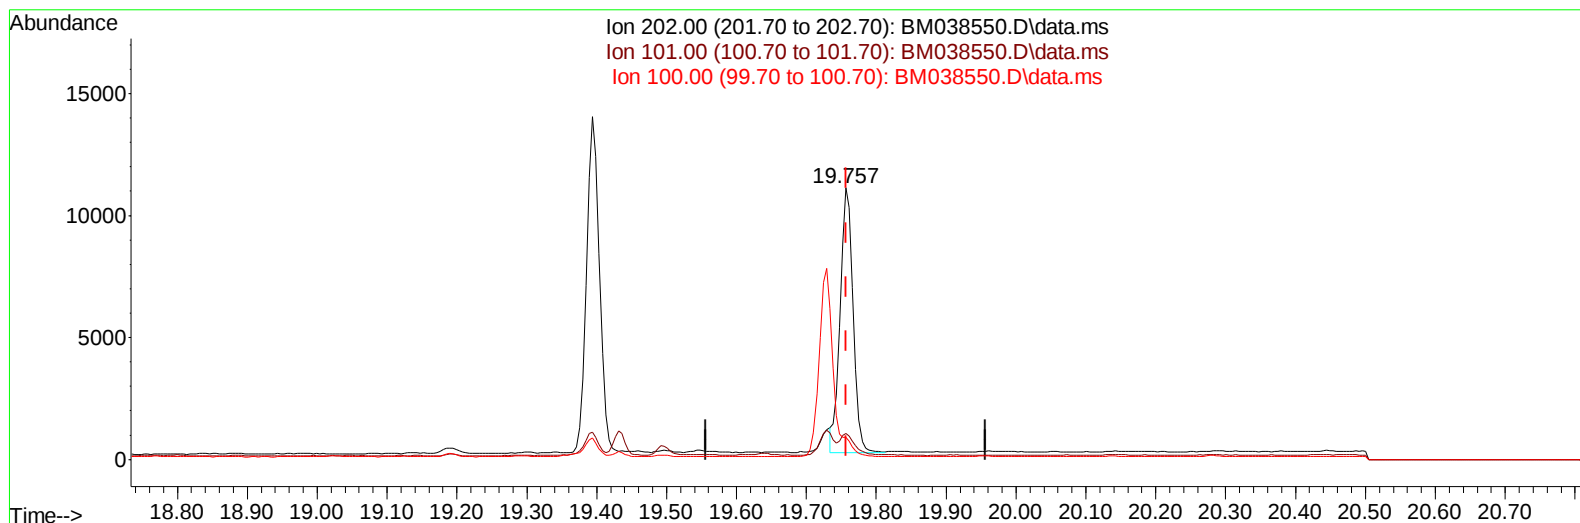

TIC: BM038550.D\data.ms

(20) Pyrene

19.757min (-0.000) 0.49 ng/u1 m

response 14179

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.40	9.56#
100.00	6.50	8.17#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038550.D
 Acq On : 26 Jan 2023 15:40
 Operator : CG/JU
 Sample : 01226-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/27/2023
 Supervised By :mohammad ahmed 01/30/2023

Quant Time: Jan 27 00:44:06 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.967	152		1660	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136		5041	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164		3491	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188		7644	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.518	240		7581	0.400	ng/ul	# 0.00
23) Perylene-d12	23.927	264		8251	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.339	96		10563	4.846	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152		1823	0.233	ng/ul	0.00
18) Fluoranthene-d10	19.366	212		6074	0.281	ng/ul	0.00
Target Compounds							
						Qvalue	
10) Acenaphthylene	14.324	152		496	0.032	ng/ul#	19
11) Acenaphthene	14.661	153		22889	1.951	ng/ul	98
12) Fluorene	15.642	166		318	0.022	ng/ul#	57
16) Anthracene	17.472	178		1294	0.061	ng/ul#	60
19) Fluoranthene	19.394	202		17740	0.656	ng/ul	97
20) Pyrene	19.757	202		14179m	0.488	ng/ul	
21) Benzo(a)anthracene	21.501	228		1098	0.041	ng/ul#	62
22) Chrysene	21.556	228		1235	0.046	ng/ul#	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038550.D
Acq On : 26 Jan 2023 15:40
Operator : CG/JU
Sample : 01226-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F8

Manual IntegrationsAPPROVED

Quant Time: Jan 27 00:44:06 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/27/2023
Supervised By :mohammad ahmed 01/30/2023

