

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038562.D
 Acq On : 26 Jan 2023 23:46
 Operator : CG/JU
 Sample : 01227-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F1

Quant Time: Jan 27 01:52:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1455	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	3462	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	2317	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	5364	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	6712	0.400	ng/ul	0.00
23) Perylene-d12	23.924	264	9305	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	7426	3.887	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1481	0.276	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	6081	0.317	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.381	88	288	0.149	ng/ul#	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038562.D
Acq On : 26 Jan 2023 23:46
Operator : CG/JU
Sample : 01227-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F1

Quant Time: Jan 27 01:52:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

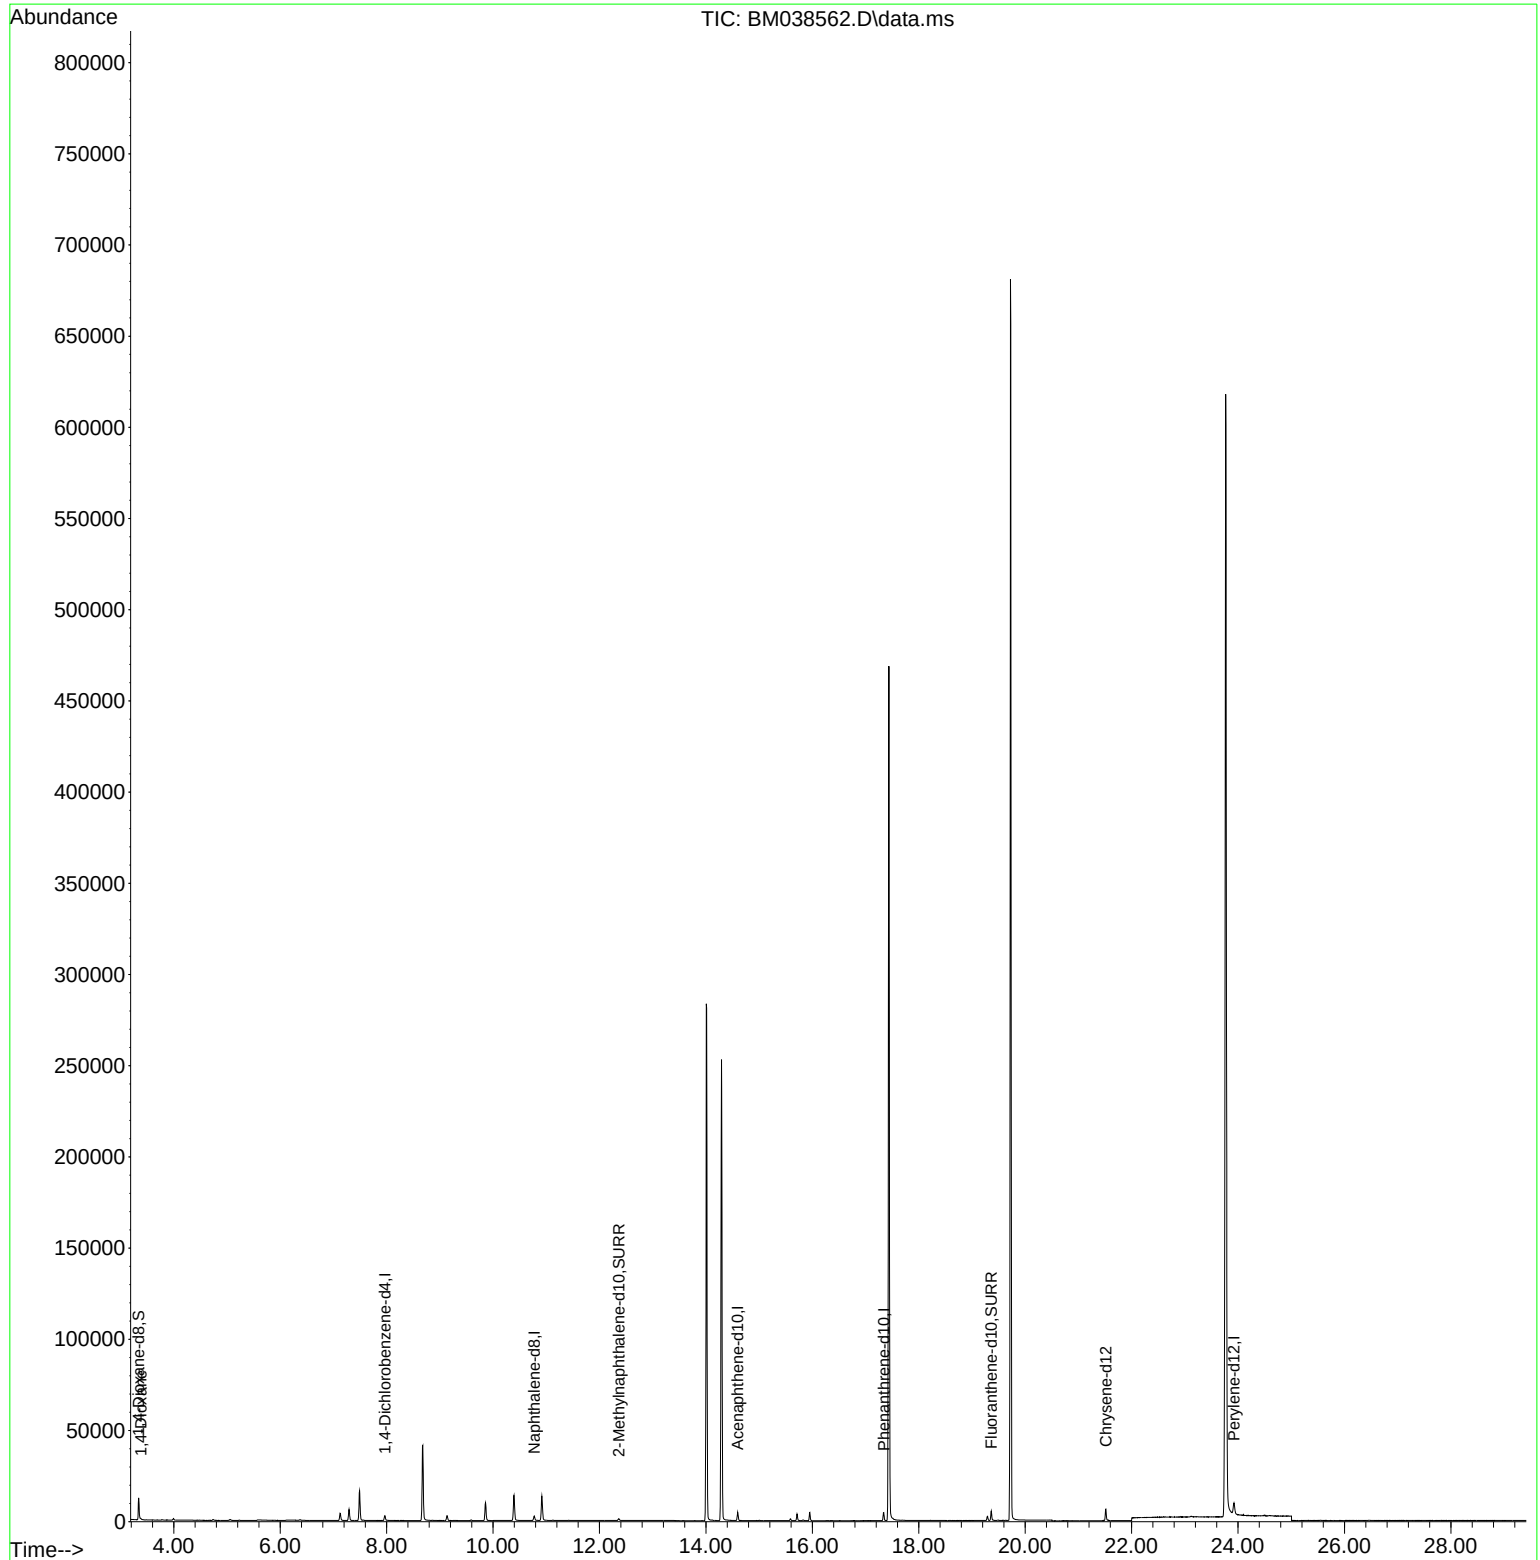

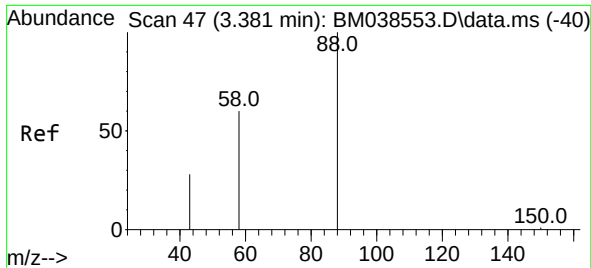

#2
 1,4-Dioxane
 Concen: 0.149 ng/ul
 RT: 3.381 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BM038562.D
 Acq: 26 Jan 2023 23:46

Instrument :
 BNA_M
 ClientSampleId :
 EX9F1

Tgt Ion: 88 Resp: 288
 Ion Ratio Lower Upper
 88 100
 43 47.3 141.3 211.9#
 58 34.7 45.7 68.5#

