

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038563.D
 Acq On : 27 Jan 2023 00:22
 Operator : CG/JU
 Sample : 01226-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F3

Quant Time: Jan 27 01:53:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	2387	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	6702	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	4071	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	9988	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	10409	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	13129	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	9842	3.140	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	2371	0.228	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	8604	0.289	ng/ul	0.00
Target Compounds						
16) Anthracene	17.472	178	800	0.029	ng/ul#	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038563.D
Acq On : 27 Jan 2023 00:22
Operator : CG/JU
Sample : 01226-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F3


Quant Time: Jan 27 01:53:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

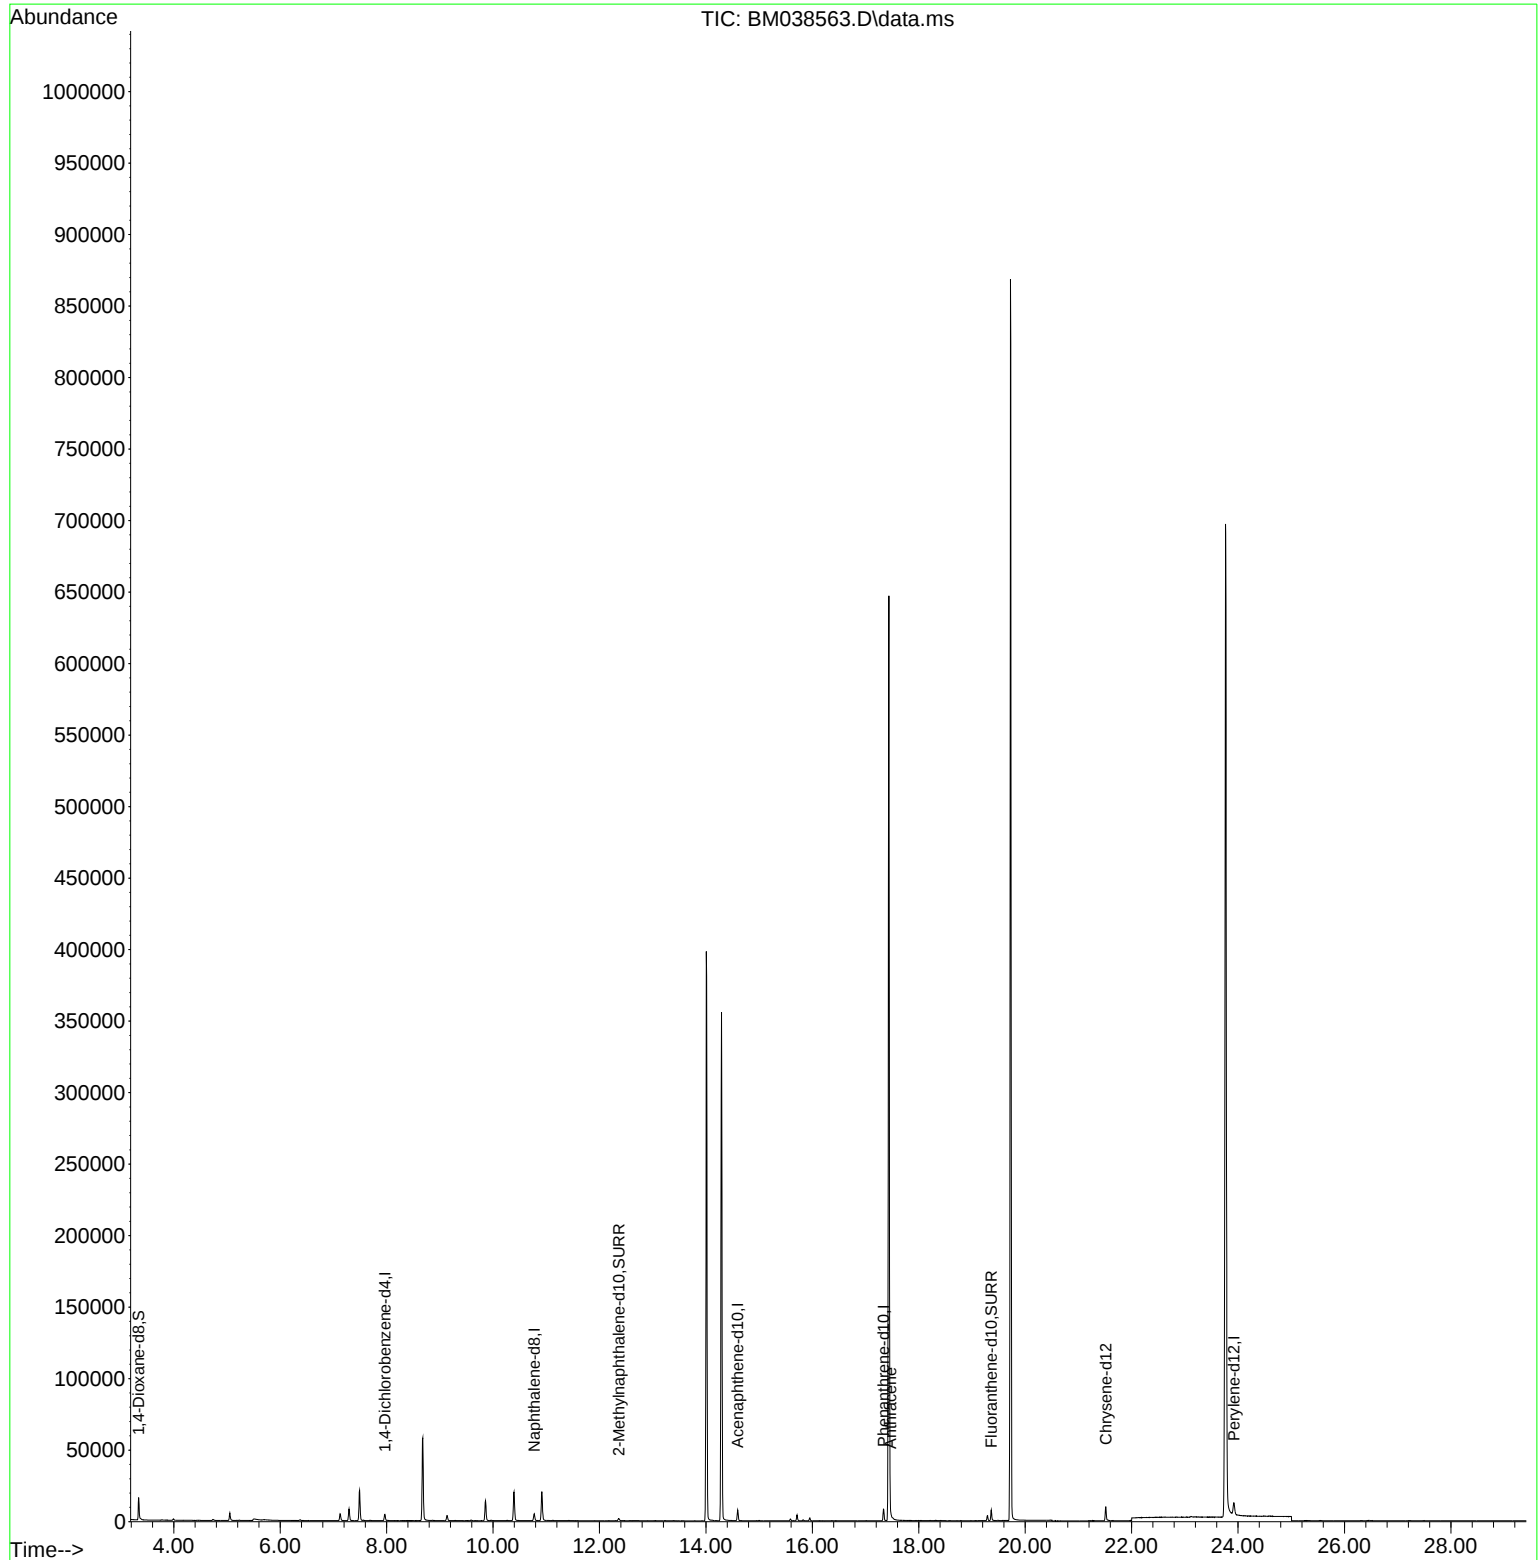

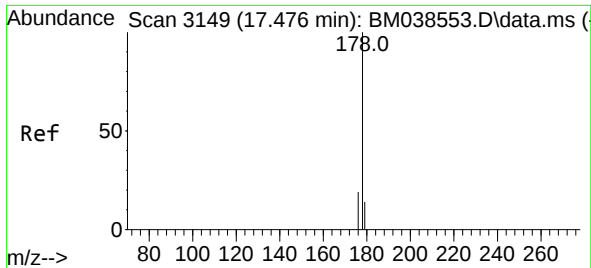

#16
 Anthracene
 Concen: 0.029 ng/ul
 RT: 17.472 min Scan# 3148
 Delta R.T. -0.004 min
 Lab File: BM038563.D
 Acq: 27 Jan 2023 00:22

Instrument :
 BNA_M
 ClientSampleId :
 EX9F3

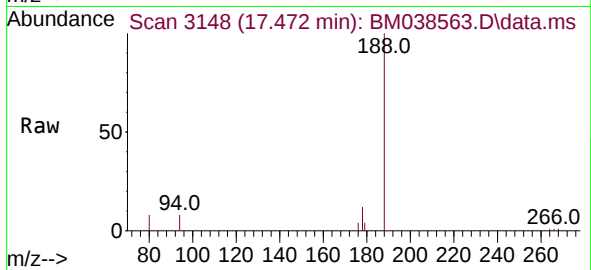

Tgt Ion:178 Resp: 800
 Ion Ratio Lower Upper
 178 100
 179 29.7 13.2 19.8#
 176 28.9 16.2 24.4#

