

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038564.D
 Acq On : 27 Jan 2023 00:59
 Operator : CG/JU
 Sample : 01227-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F3

Quant Time: Jan 27 01:54:10 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	2055	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	5484	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	3494	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	7675	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	8042	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	9940	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.338	96	10868	4.027	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	2101	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	7868	0.343	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.381	88	388	0.142	ng/ul#	25

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\  
Data File : BM038564.D  
Acq On    : 27 Jan 2023   00:59  
Operator  : CG/JU  
Sample    : 01227-02  
Misc      :  
ALS Vial  : 22      Sample Multiplier: 1
```

Quant Time: Jan 27 01:54:10 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

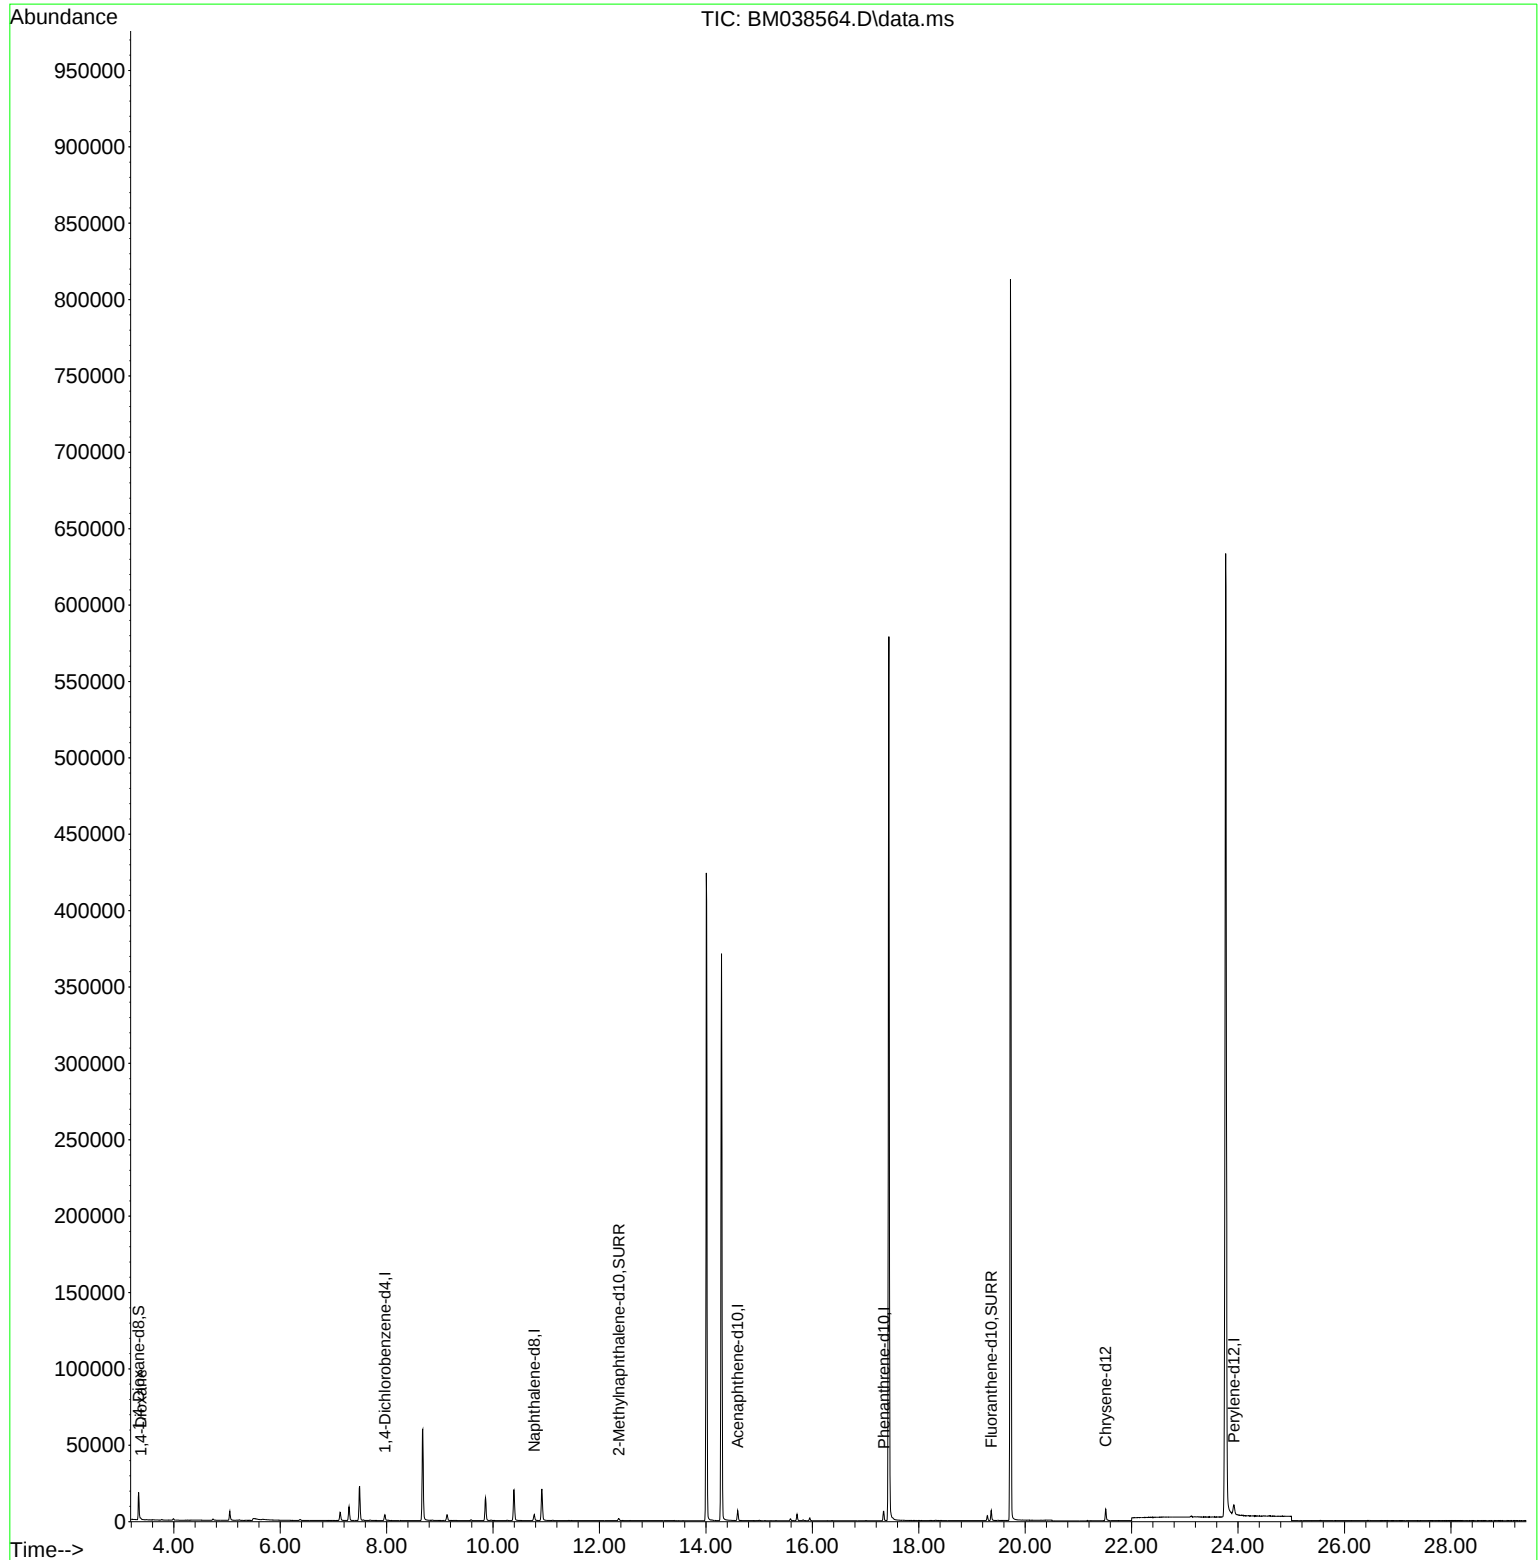

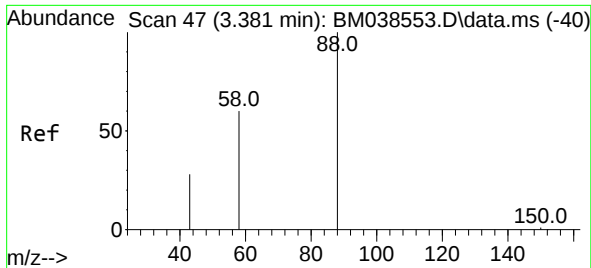

#2
 1,4-Dioxane
 Concen: 0.142 ng/ul
 RT: 3.381 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BM038564.D
 Acq: 27 Jan 2023 00:59

Instrument :
 BNA_M
 ClientSampleId :
 EX9F3

Tgt Ion: 88 Resp: 388
 Ion Ratio Lower Upper
 88 100
 43 52.6 141.3 211.9#
 58 31.1 45.7 68.5#

