

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038567.D
 Acq On : 27 Jan 2023 02:49
 Operator : CG/JU
 Sample : 01226-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F5

Quant Time: Jan 27 03:58:04 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	2093	0.400	ng/u1	0.00
4) Naphthalene-d8	10.774	136	5742	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.597	164	3876	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.337	188	7857	0.400	ng/u1	0.00
17) Chrysene-d12	21.512	240	7670	0.400	ng/u1	0.00
23) Perylene-d12	23.921	264	9473	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	8218	2.990	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.357	152	2264	0.254	ng/u1	0.00
18) Fluoranthene-d10	19.362	212	7442	0.340	ng/u1	0.00
Target Compounds						
16) Anthracene	17.472	178	633	0.029	ng/u1#	Qvalue 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038567.D
Acq On : 27 Jan 2023 02:49
Operator : CG/JU
Sample : 01226-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F5


Quant Time: Jan 27 03:58:04 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

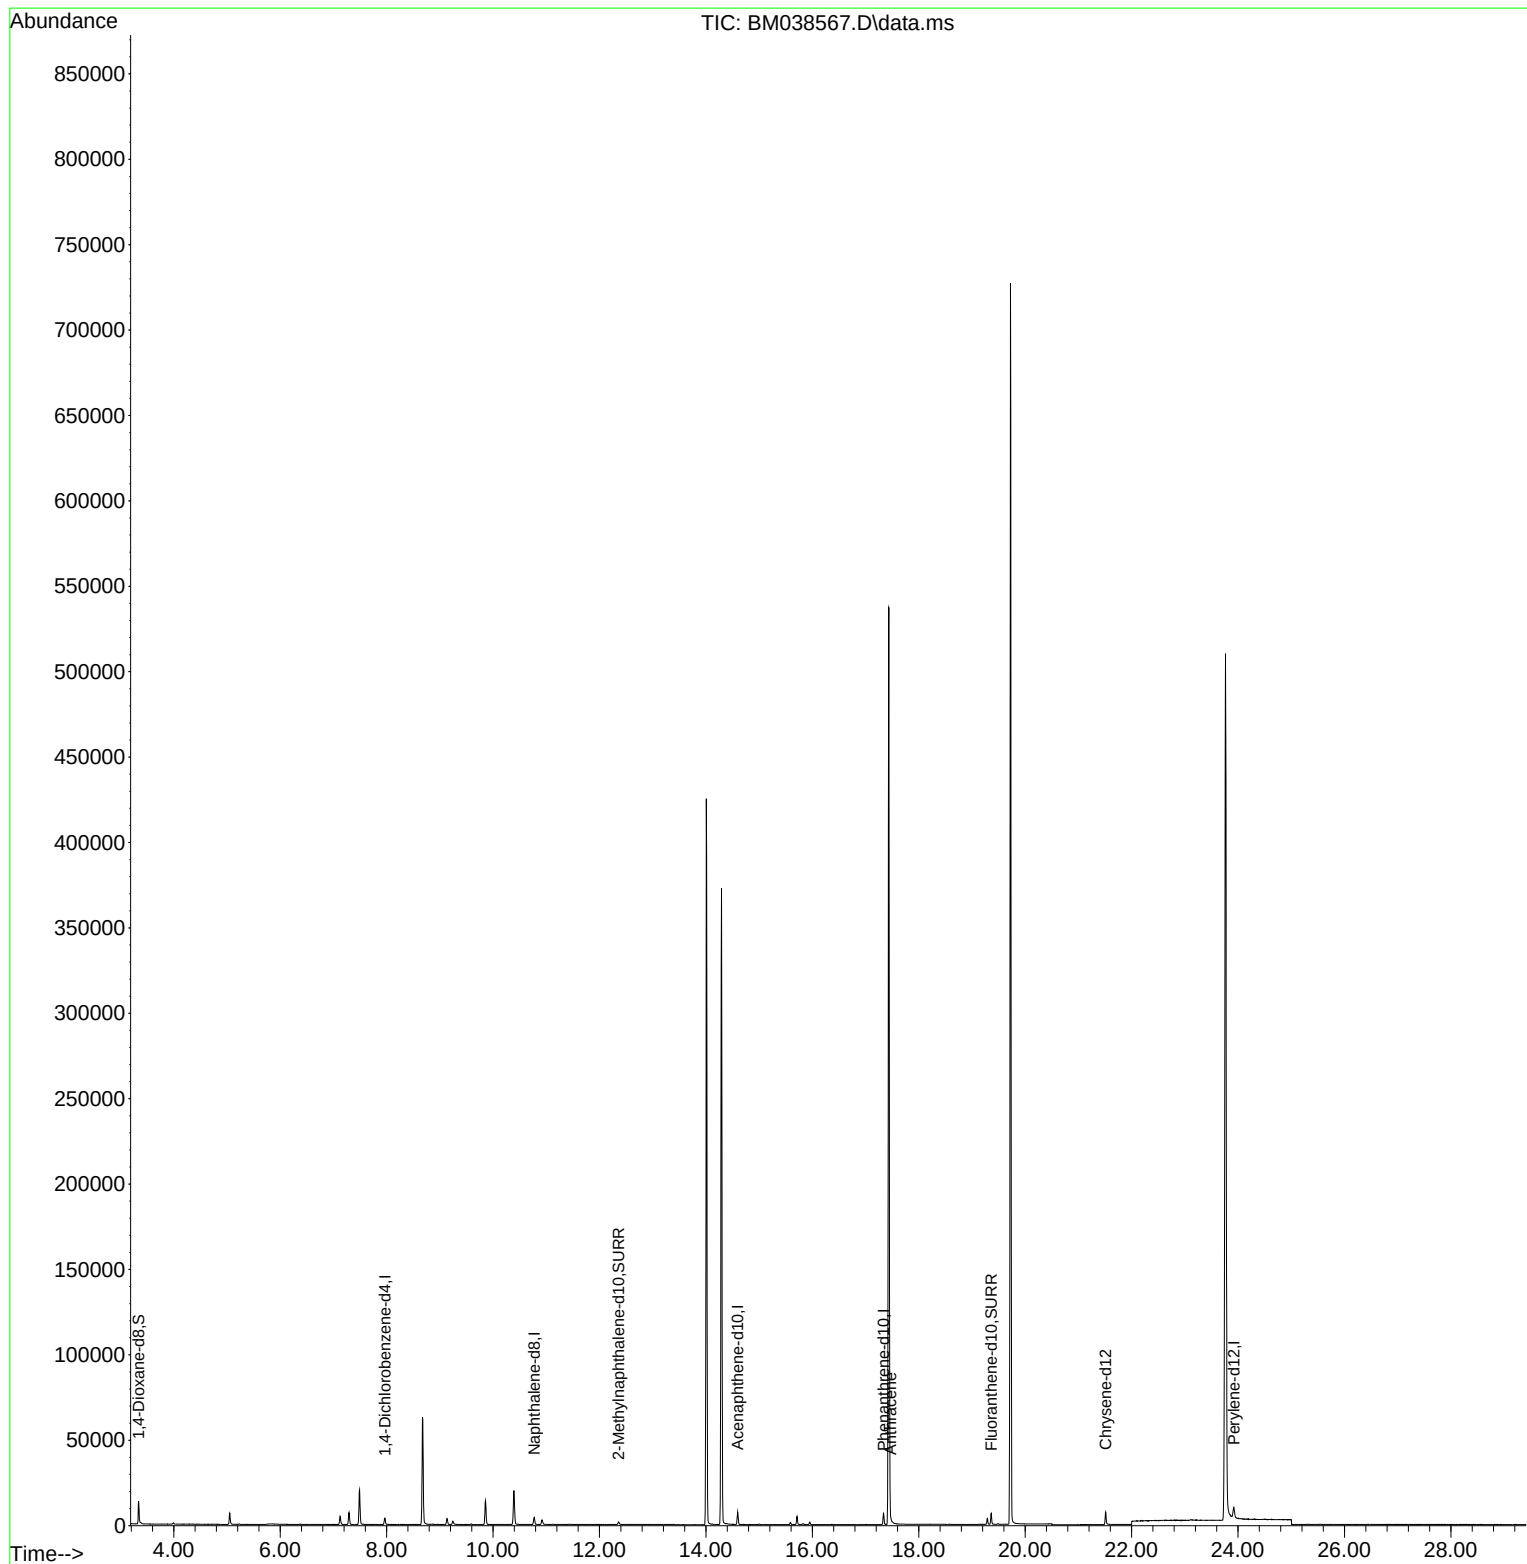

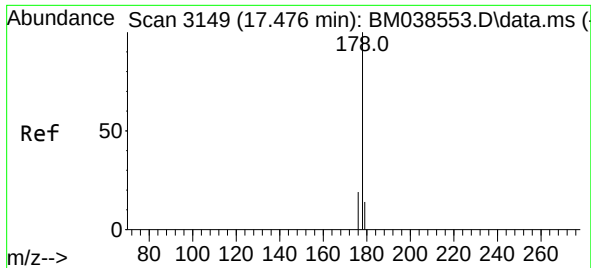

#16
 Anthracene
 Concen: 0.029 ng/ul
 RT: 17.472 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BM038567.D
 Acq: 27 Jan 2023 02:49

Instrument :
 BNA_M
 ClientSampleId :
 EX9F5

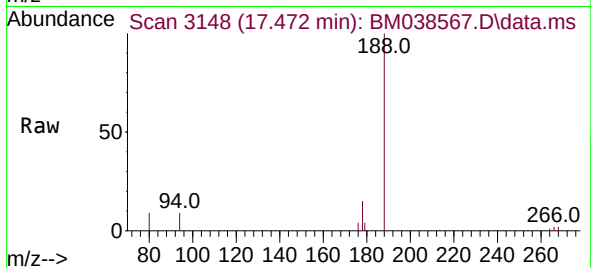

Tgt Ion:	178	Resp:	633
Ion	Ratio	Lower	Upper
178	100		
179	30.3	13.2	19.8#
176	29.5	16.2	24.4#

