

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038568.D
 Acq On : 27 Jan 2023 03:25
 Operator : CG/JU
 Sample : 01227-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F5

Quant Time: Jan 27 03:58:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1981	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	5430	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	3675	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	7745	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	7498	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	10212	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.338	96	7712	2.965	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	2566	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	8937	0.417	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.376	88	350	0.133	ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038568.D
Acq On : 27 Jan 2023 03:25
Operator : CG/JU
Sample : 01227-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F5

Quant Time: Jan 27 03:58:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

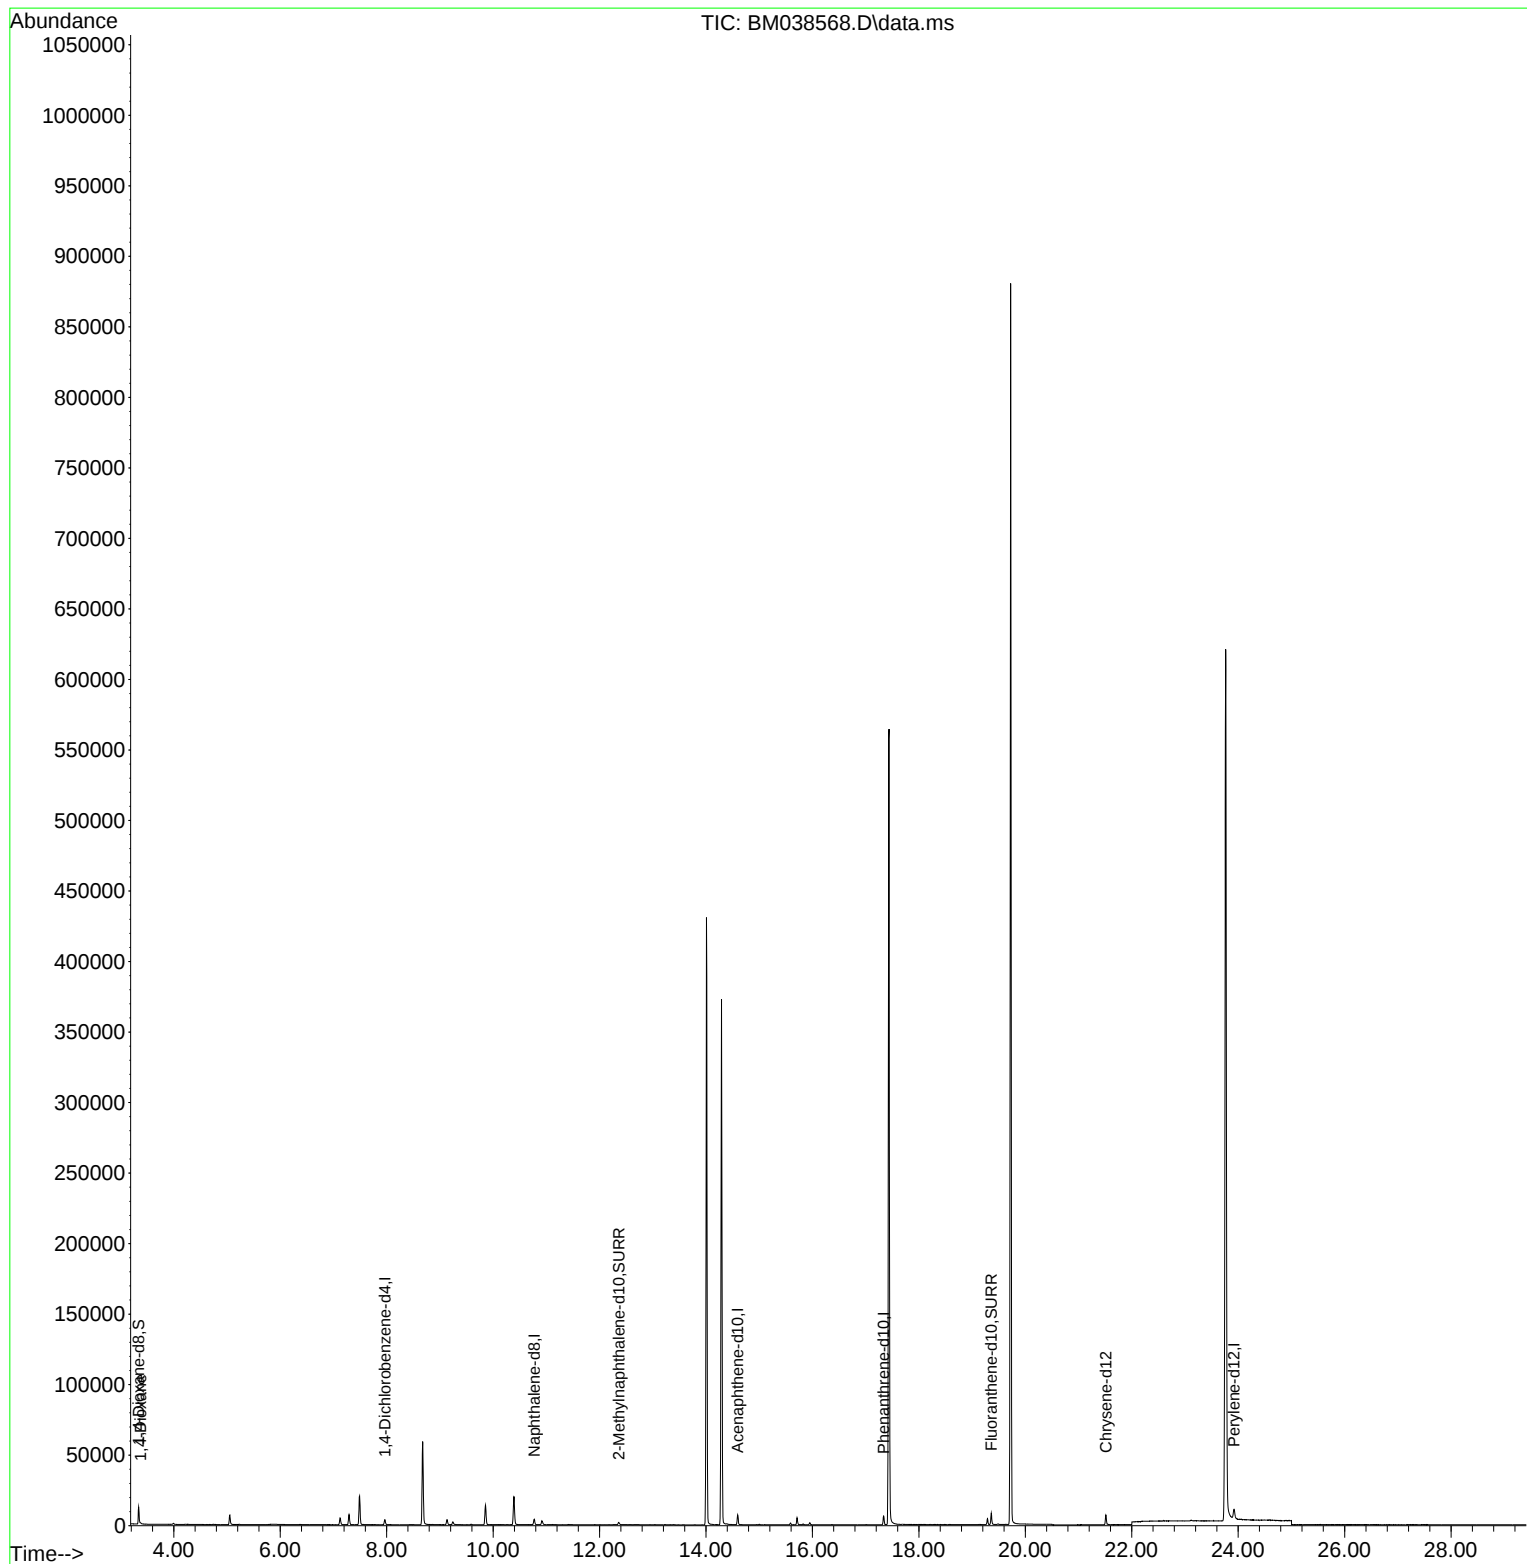

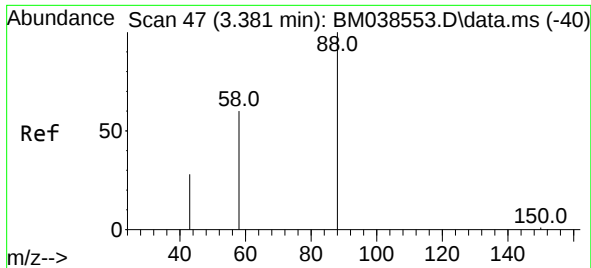

#2
 1,4-Dioxane
 Concen: 0.133 ng/ul
 RT: 3.376 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BM038568.D
 Acq: 27 Jan 2023 03:25

Instrument :
 BNA_M
 ClientSampleId :
 EX9F5

Tgt Ion: 88 Resp: 350
 Ion Ratio Lower Upper
 88 100
 43 49.9 141.3 211.9#
 58 33.8 45.7 68.5#

