

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038569.D
 Acq On : 27 Jan 2023 04:02
 Operator : CG/JU
 Sample : 01226-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F6

Quant Time: Jan 27 04:36:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1626	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	4466	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	2785	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	5895	0.400	ng/ul	0.00
17) Chrysene-d12	21.513	240	6719	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	8633	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	5860	2.744	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	1747	0.252	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	5571	0.290	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.390	202	557	0.023	ng/ul#	Qvalue 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038569.D
Acq On : 27 Jan 2023 04:02
Operator : CG/JU
Sample : 01226-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F6


Quant Time: Jan 27 04:36:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

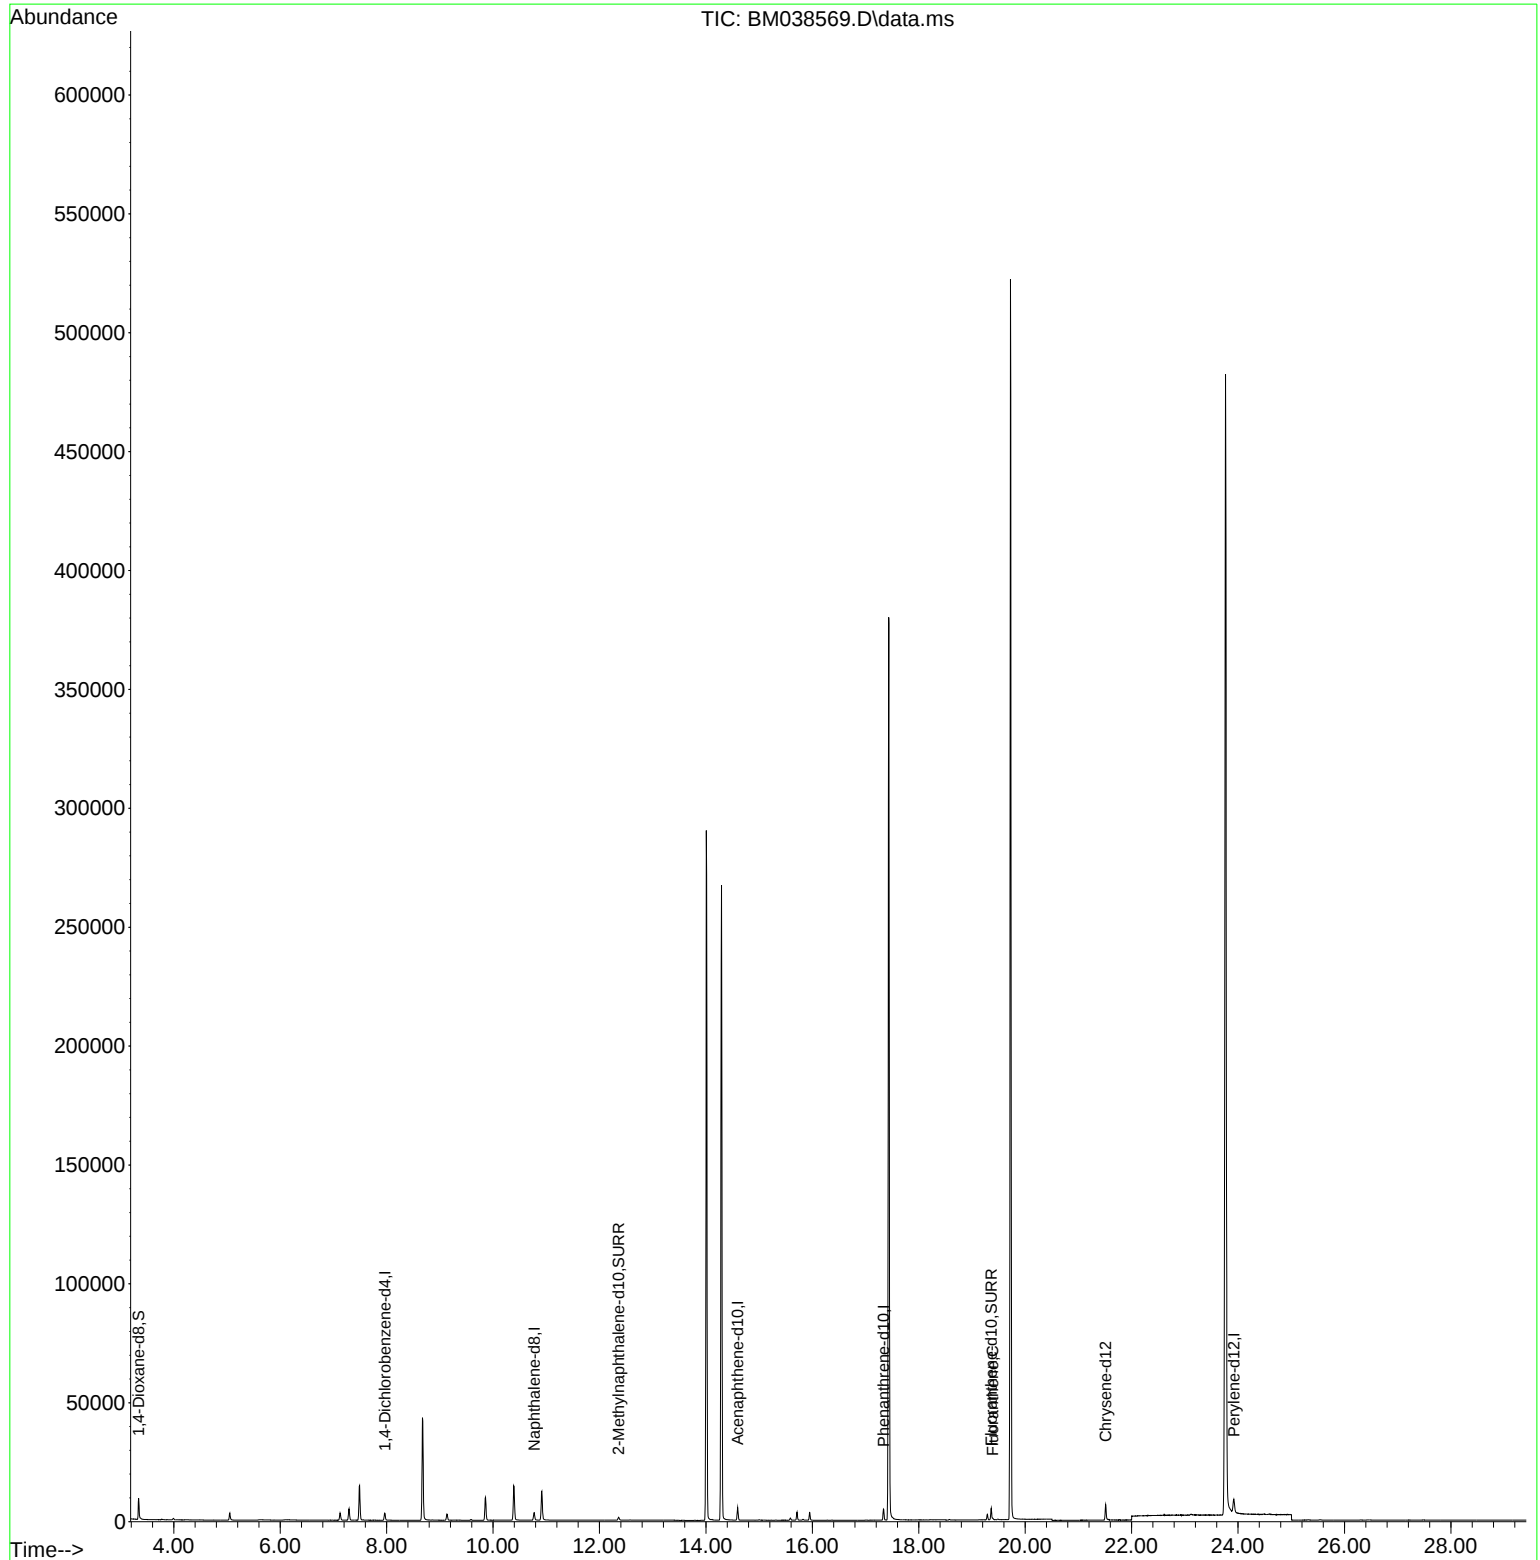

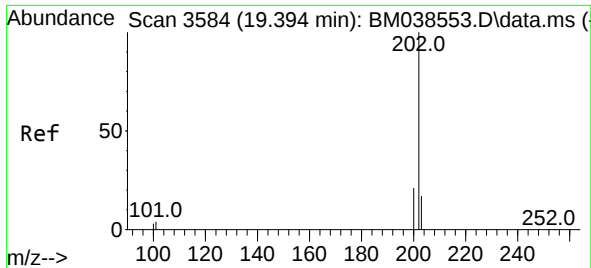

#19
 Fluoranthene
 Concen: 0.023 ng/ul
 RT: 19.390 min Scan# 31
 Delta R.T. -0.005 min
 Lab File: BM038569.D
 Acq: 27 Jan 2023 04:02

Instrument :
 BNA_M
 ClientSampleId :
 EX9F6

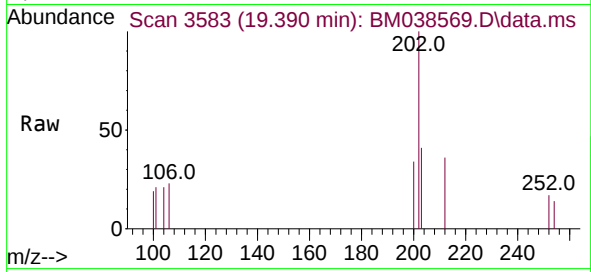

Tgt Ion:202 Resp: 557
 Ion Ratio Lower Upper
 202 100
 101 21.2 5.3 7.9#
 100 19.0 4.2 6.2#

