

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038577.D
 Acq On : 27 Jan 2023 09:29
 Operator : CG/JU
 Sample : 01227-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F8

Quant Time: Jan 27 21:58:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	1960	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	5752	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.597	164	3881	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	8098	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.512	240	7523	0.400	ng/ul	# 0.00
23) Perylene-d12	23.921	264	8031	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	9237	3.589	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	2160	0.242	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	6797	0.316	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.376	88	449	0.172	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038577.D
Acq On : 27 Jan 2023 09:29
Operator : CG/JU
Sample : 01227-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F8

Quant Time: Jan 27 21:58:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

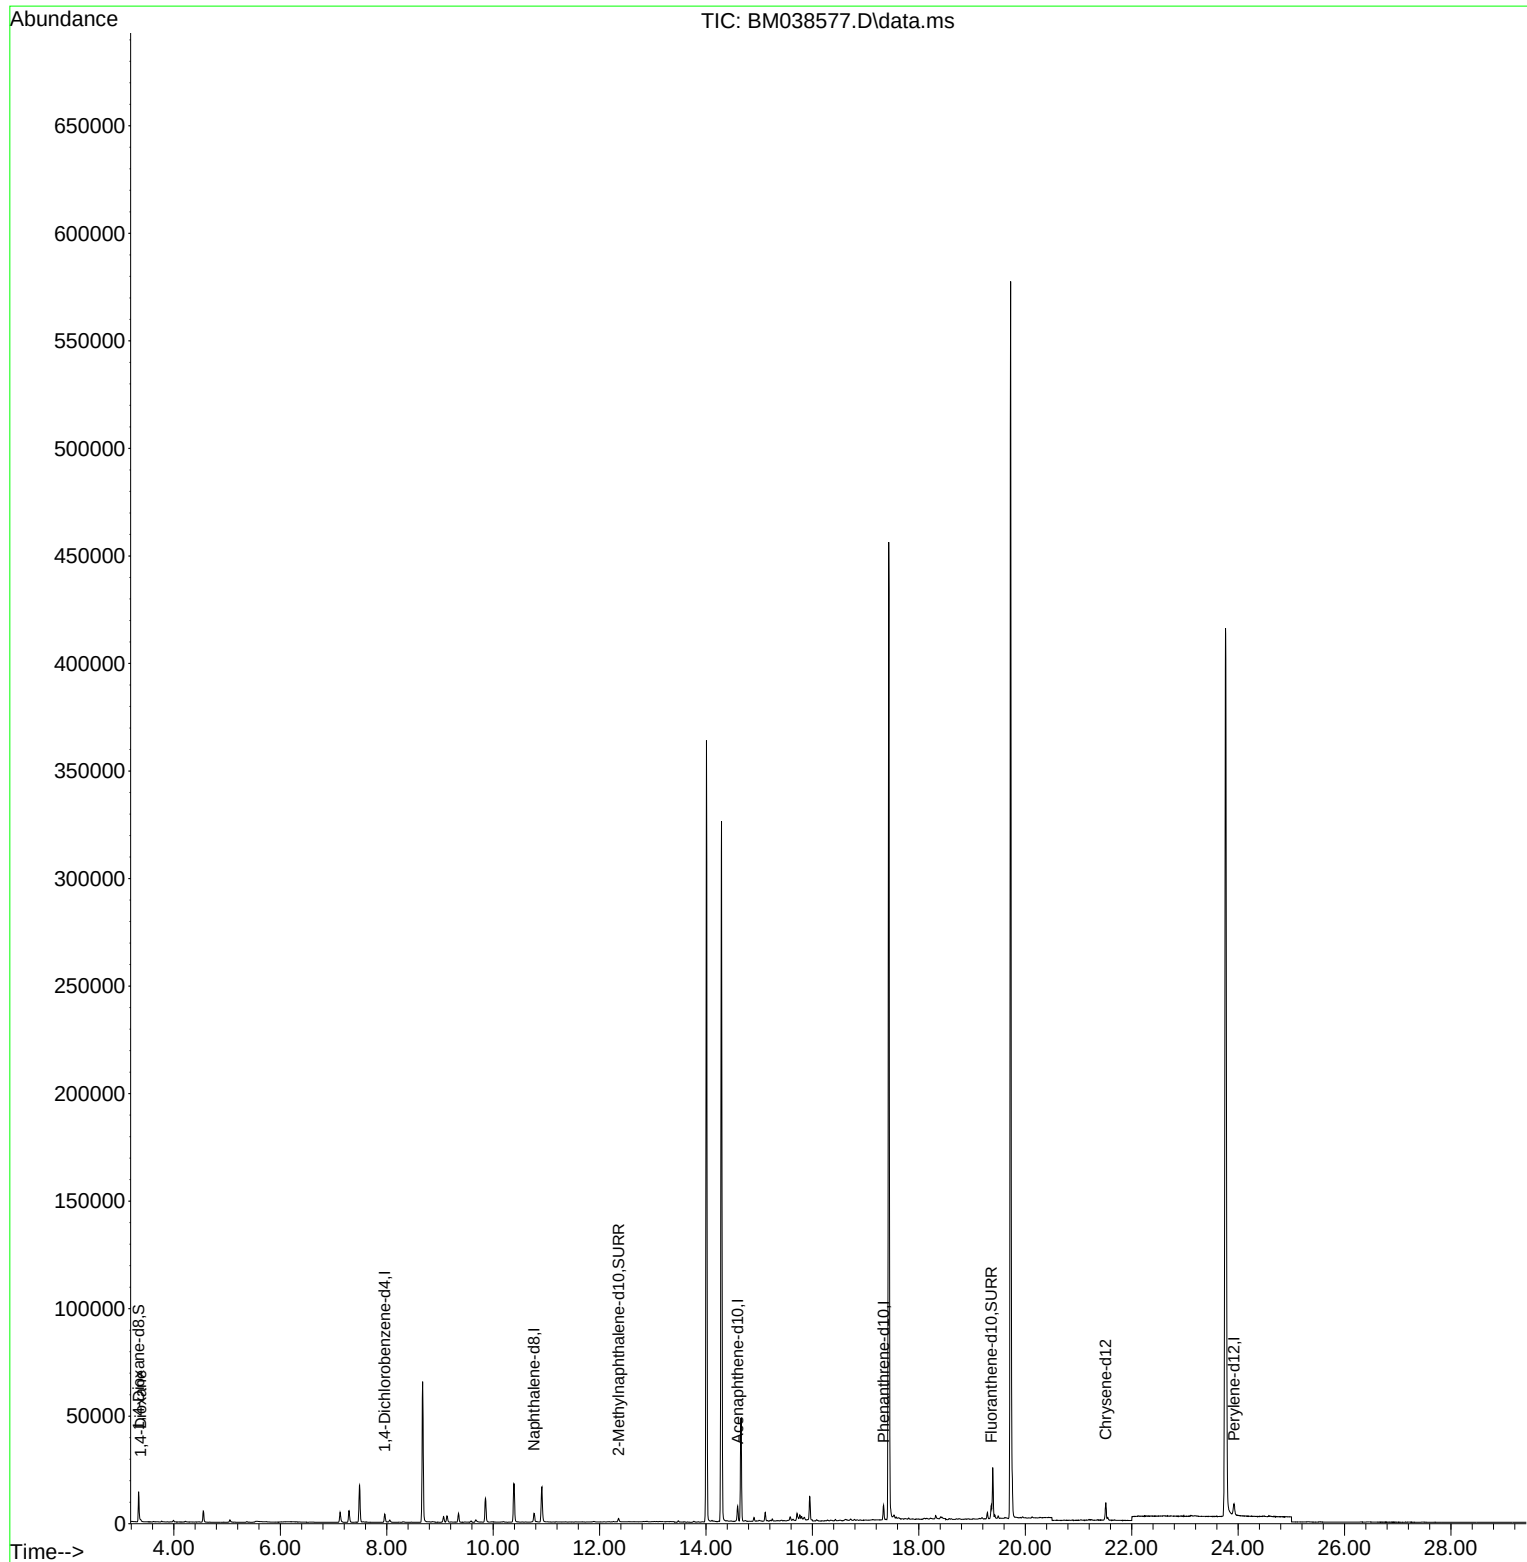

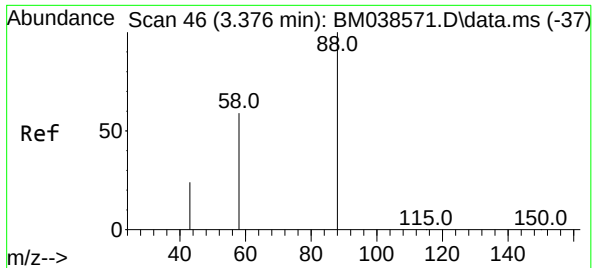

#2
 1,4-Dioxane
 Concen: 0.172 ng/ul
 RT: 3.376 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BM038577.D
 Acq: 27 Jan 2023 09:29

Instrument :
 BNA_M
 ClientSampleId :
 EX9F8

Tgt Ion:	88	Resp:	449
Ion	Ratio	Lower	Upper
88	100		
43	59.2	141.3	211.9#
58	48.4	45.7	68.5

