

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038582.D
 Acq On : 27 Jan 2023 12:34
 Operator : CG/JU
 Sample : 01226-02
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F3

Quant Time: Jan 27 21:59:31 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1115	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	3176	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.597	164	2122	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	4633	0.400	ng/ul	0.00
17) Chrysene-d12	21.516	240	5215	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	6710	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	5619	3.838	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.358	152	1428	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	4577	0.307	ng/ul	0.00
Target Compounds						
16) Anthracene	17.472	178	313	0.025	ng/ul#	Qvalue 54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038582.D
Acq On : 27 Jan 2023 12:34
Operator : CG/JU
Sample : 01226-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F3


Quant Time: Jan 27 21:59:31 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

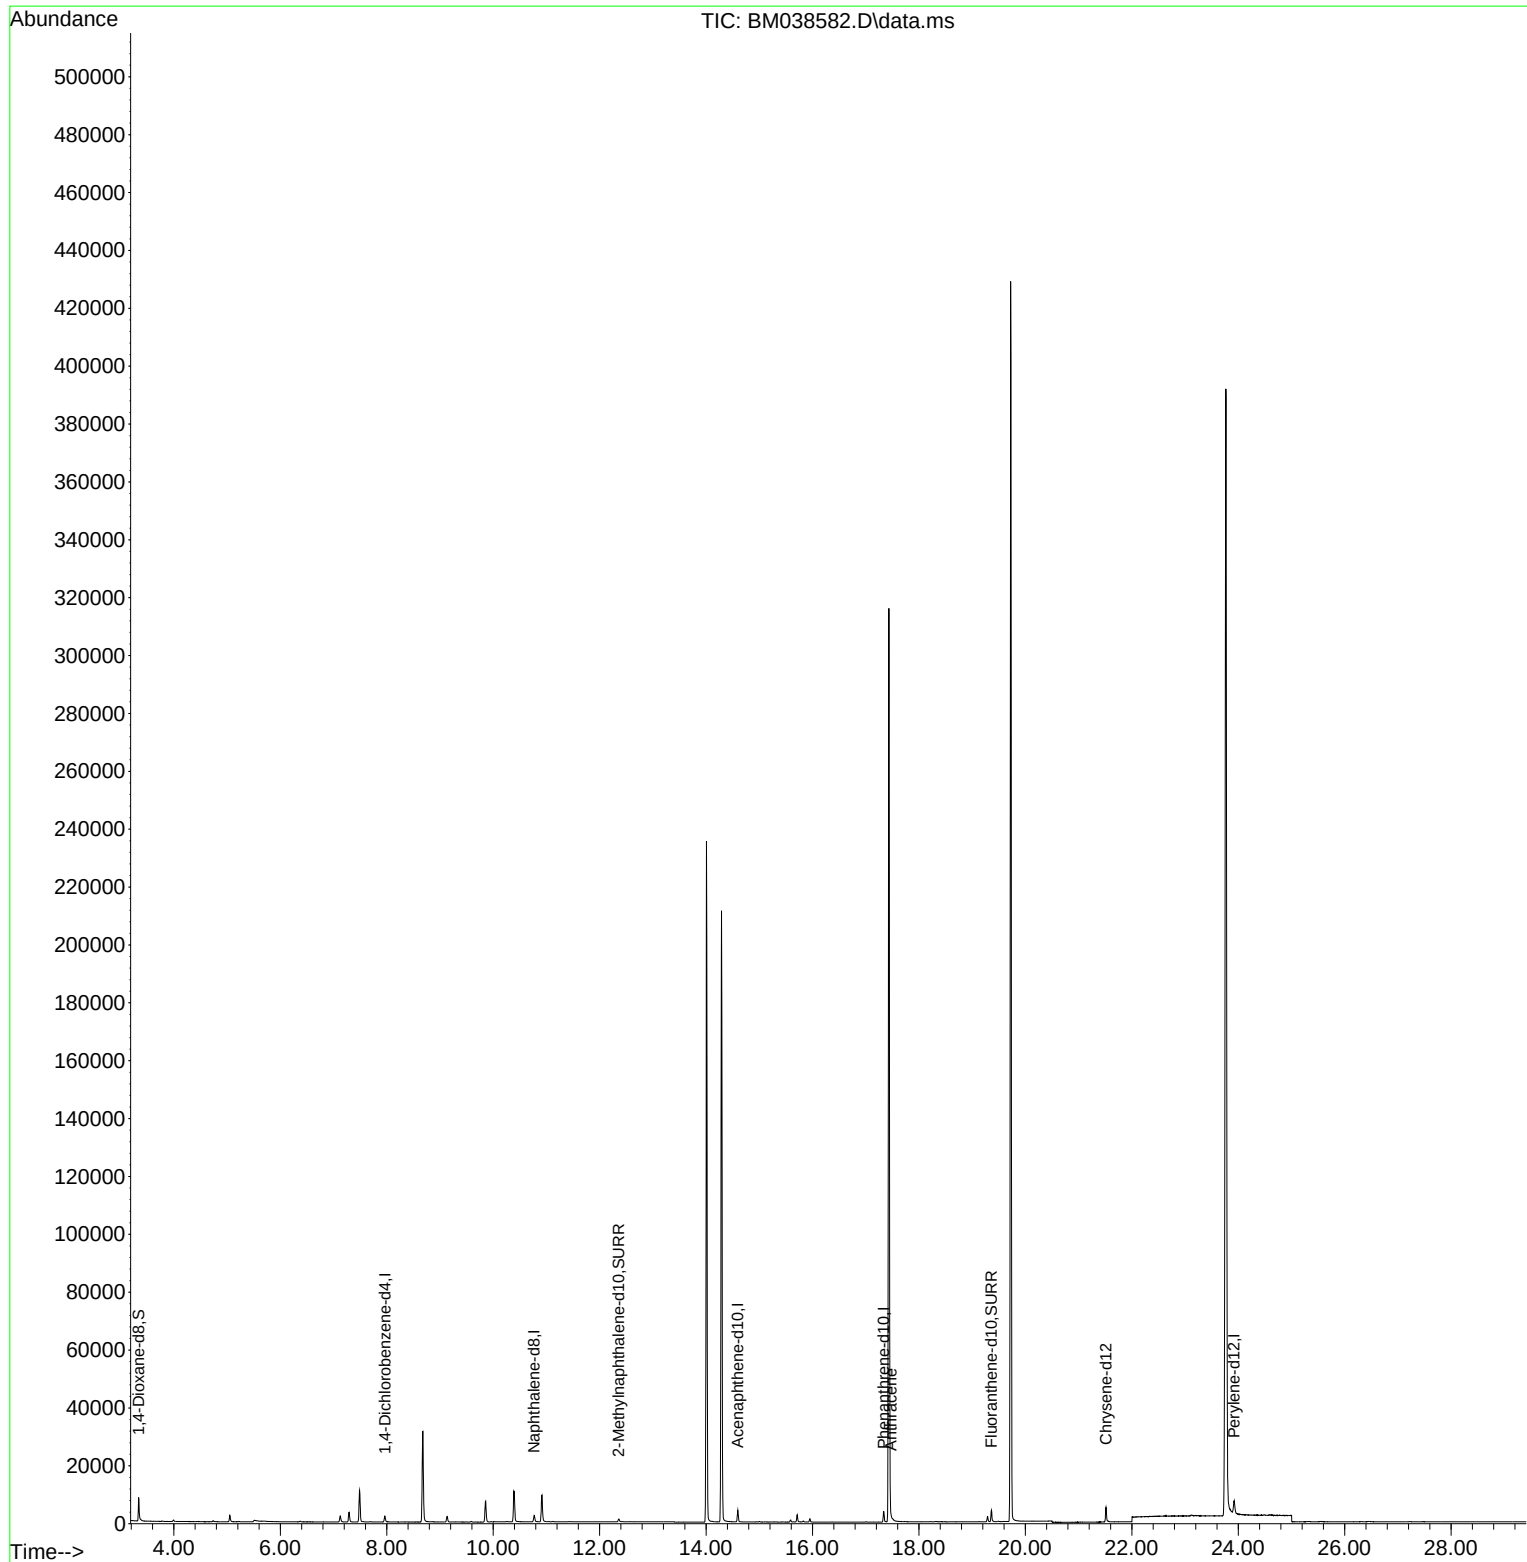

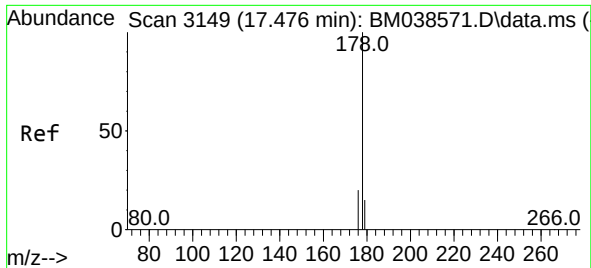

#16
 Anthracene
 Concen: 0.025 ng/ul
 RT: 17.472 min Scan# 3148
 Delta R.T. -0.004 min
 Lab File: BM038582.D
 Acq: 27 Jan 2023 12:34

Instrument :
 BNA_M
 ClientSampleId :
 EX9F3

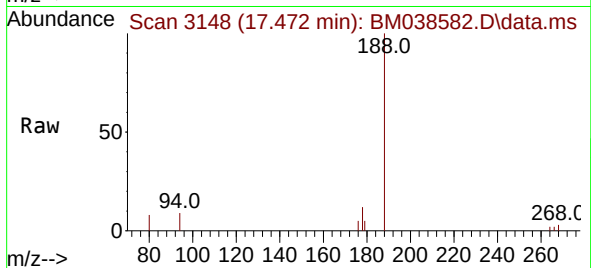

Tgt Ion:178 Resp: 313
 Ion Ratio Lower Upper
 178 100
 179 40.2 13.2 19.8#
 176 38.2 16.2 24.4#

