

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038591.D
 Acq On : 27 Jan 2023 18:45
 Operator : CG/JU
 Sample : 01226-11
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9G5

Quant Time: Jan 27 22:00:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1564	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	4225	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.597	164	2617	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	5483	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	5752	0.400	ng/ul	# 0.00
23) Perylene-d12	23.918	264	7209	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.338	96	7354	3.581	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	1442	0.220	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	4430	0.270	ng/ul	0.00
Target Compounds						
16) Anthracene	17.468	178	842	0.056	ng/ul#	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038591.D
Acq On : 27 Jan 2023 18:45
Operator : CG/JU
Sample : 01226-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G5


Quant Time: Jan 27 22:00:52 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

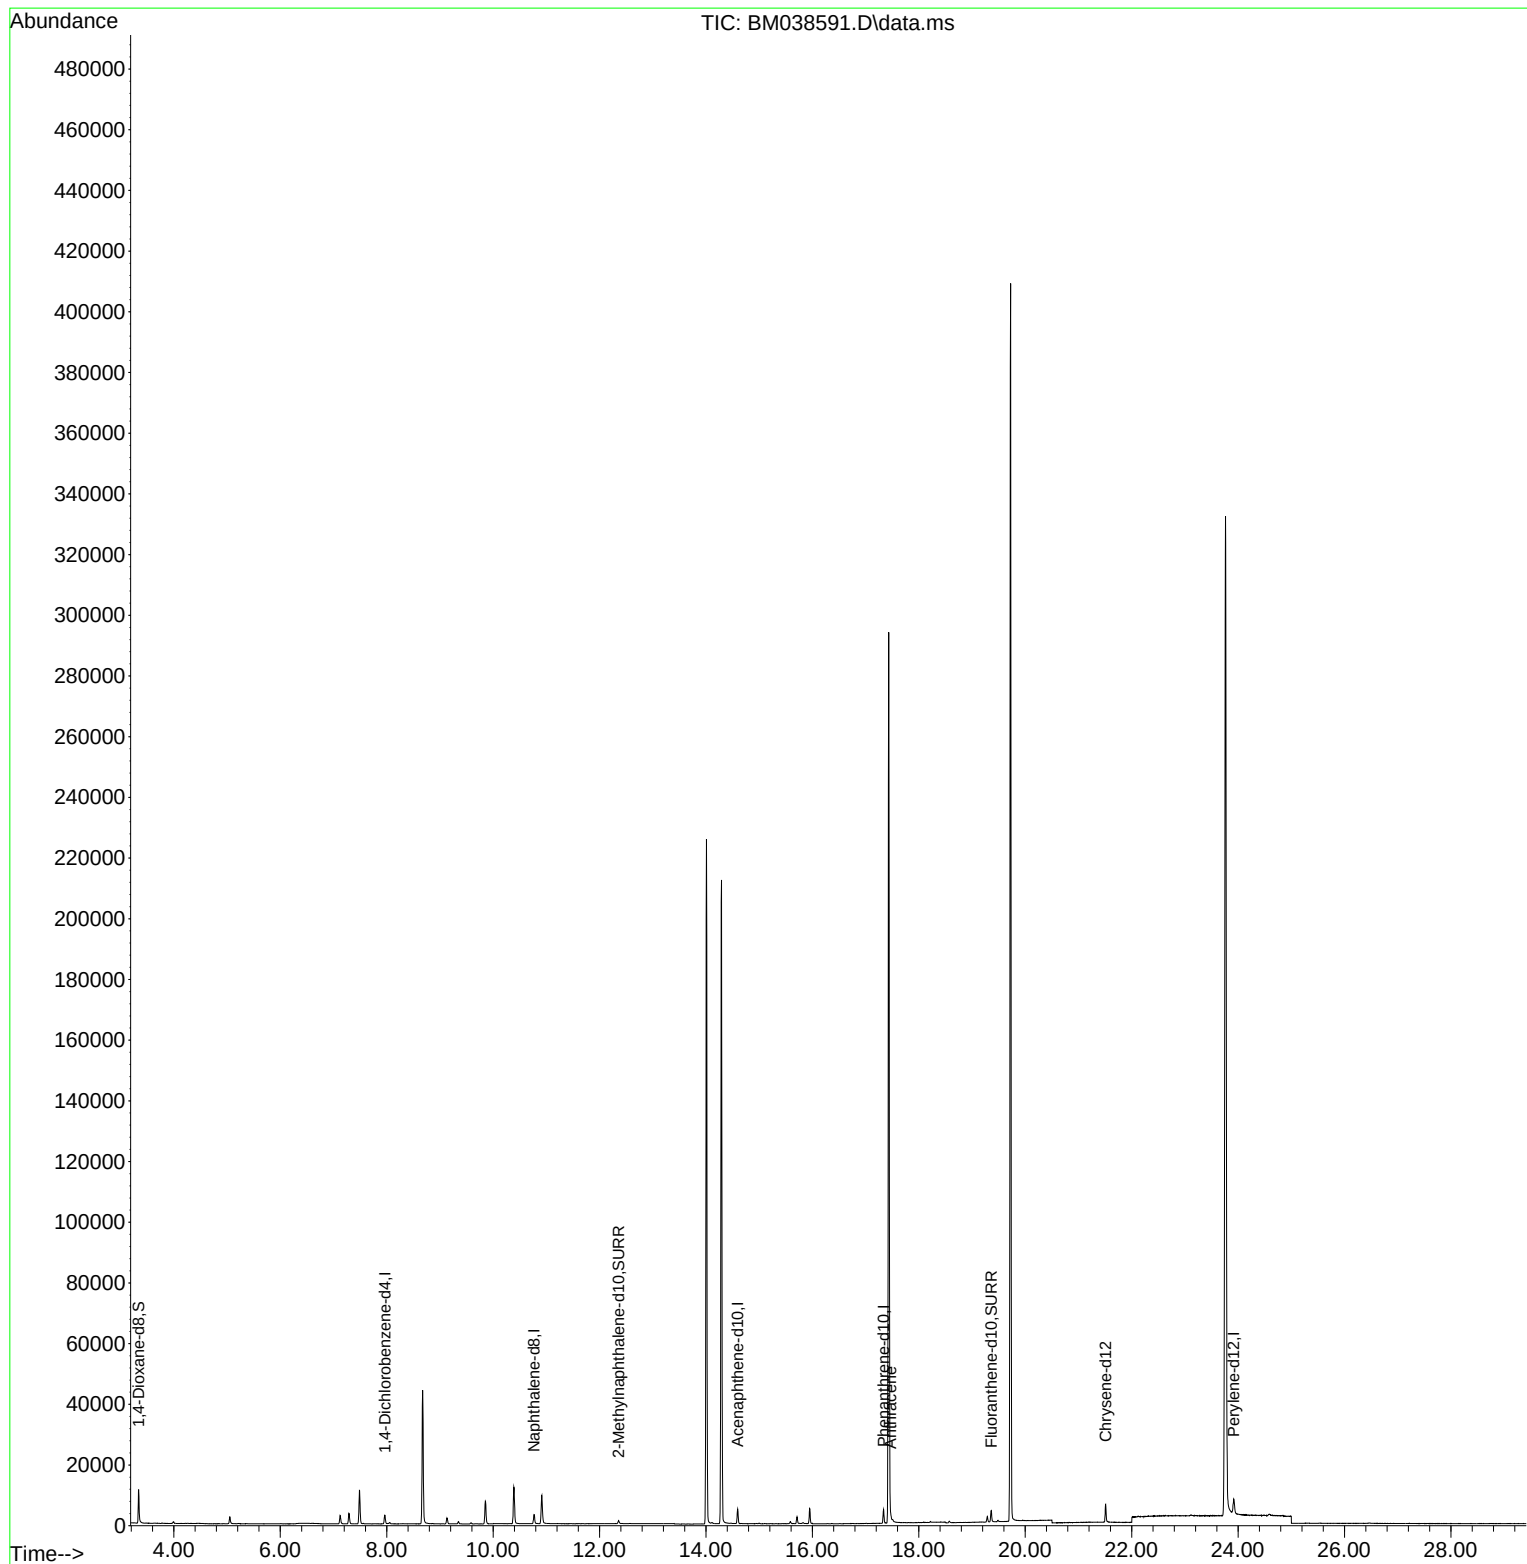

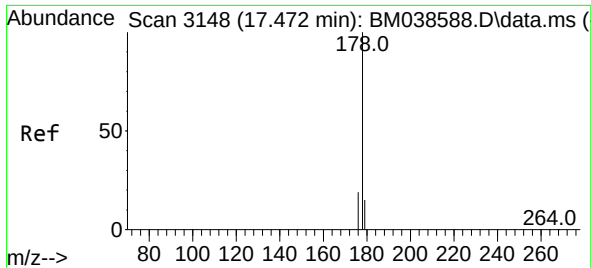

#16
 Anthracene
 Concen: 0.056 ng/ul
 RT: 17.468 min Scan# 3147
 Delta R.T. -0.009 min
 Lab File: BM038591.D
 Acq: 27 Jan 2023 18:45

Instrument :
 BNA_M
 ClientSampleId :
 EX9G5

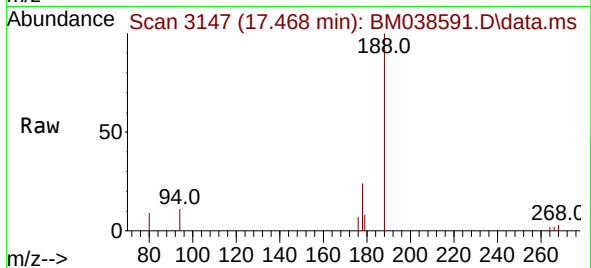

Tgt Ion	Ratio	Lower	Upper
178	100		
179	32.9	13.2	19.8#
176	31.6	16.2	24.4#

