

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038593.D
 Acq On : 27 Jan 2023 19:59
 Operator : CG/JU
 Sample : 01226-12
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9F9

Quant Time: Jan 27 22:01:05 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	1651	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	4705	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.597	164	3300	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	6896	0.400	ng/ul	0.00
17) Chrysene-d12	21.510	240	6348	0.400	ng/ul	# 0.00
23) Perylene-d12	23.918	264	7011	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	7196	3.319	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	1838	0.252	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	5448	0.301	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.390	202	736	0.033	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038593.D
Acq On : 27 Jan 2023 19:59
Operator : CG/JU
Sample : 01226-12
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9F9

Quant Time: Jan 27 22:01:05 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration

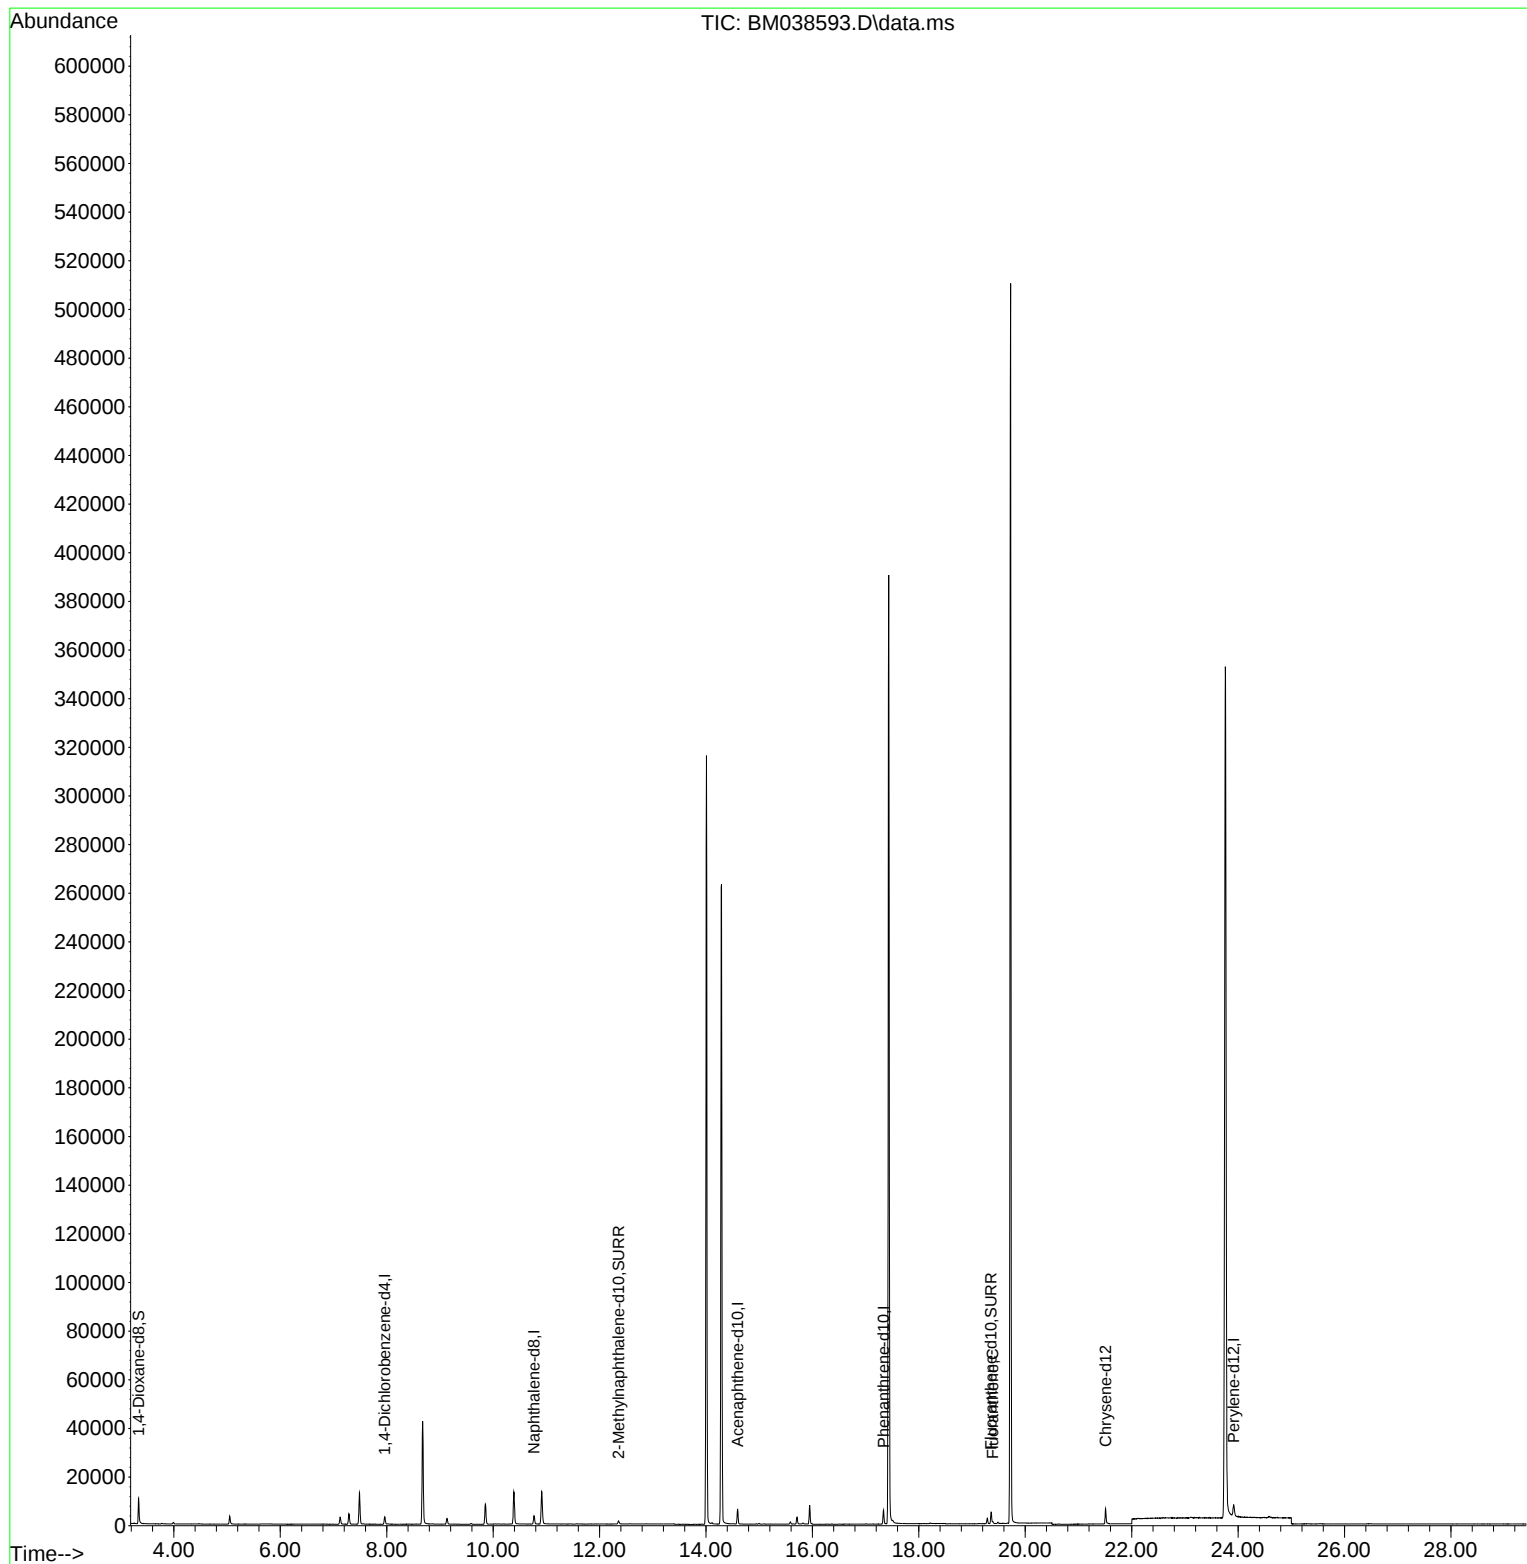

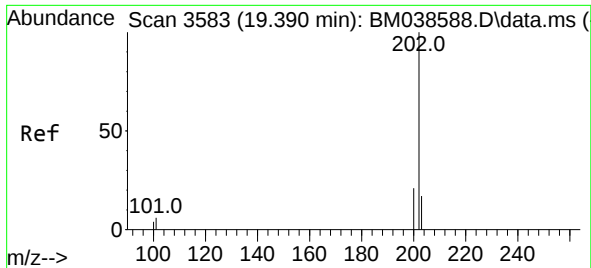

#19

Fluoranthene

Concen: 0.033 ng/ul

RT: 19.390 min Scan# 3

Delta R.T. -0.005 min

Lab File: BM038593.D


Acq: 27 Jan 2023 19:59

Instrument :

BNA_M

ClientSampleId :

EX9F9

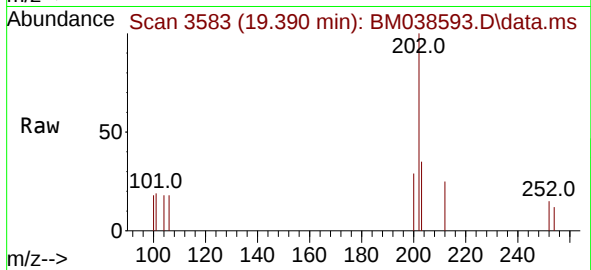

Tgt Ion:202 Resp: 736

Ion Ratio Lower Upper

202 100

101 19.4 5.3 7.9#

100 17.6 4.2 6.2#

