

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038597.D
 Acq On : 27 Jan 2023 22:26
 Operator : CG/JU
 Sample : 01226-14
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9G1

Quant Time: Jan 27 23:05:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	1116	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	3751	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.592	164	3562	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	8350	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	7711	0.400	ng/ul	0.00
23) Perylene-d12	23.918	264	7612	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.338	96	6913	4.717	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	1718	0.295	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	8093	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.389	202	1909	0.069	ng/ul#	86
20) Pyrene	19.752	202	1478	0.050	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038597.D
Acq On : 27 Jan 2023 22:26
Operator : CG/JU
Sample : 01226-14
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G1

Quant Time: Jan 27 23:05:52 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration




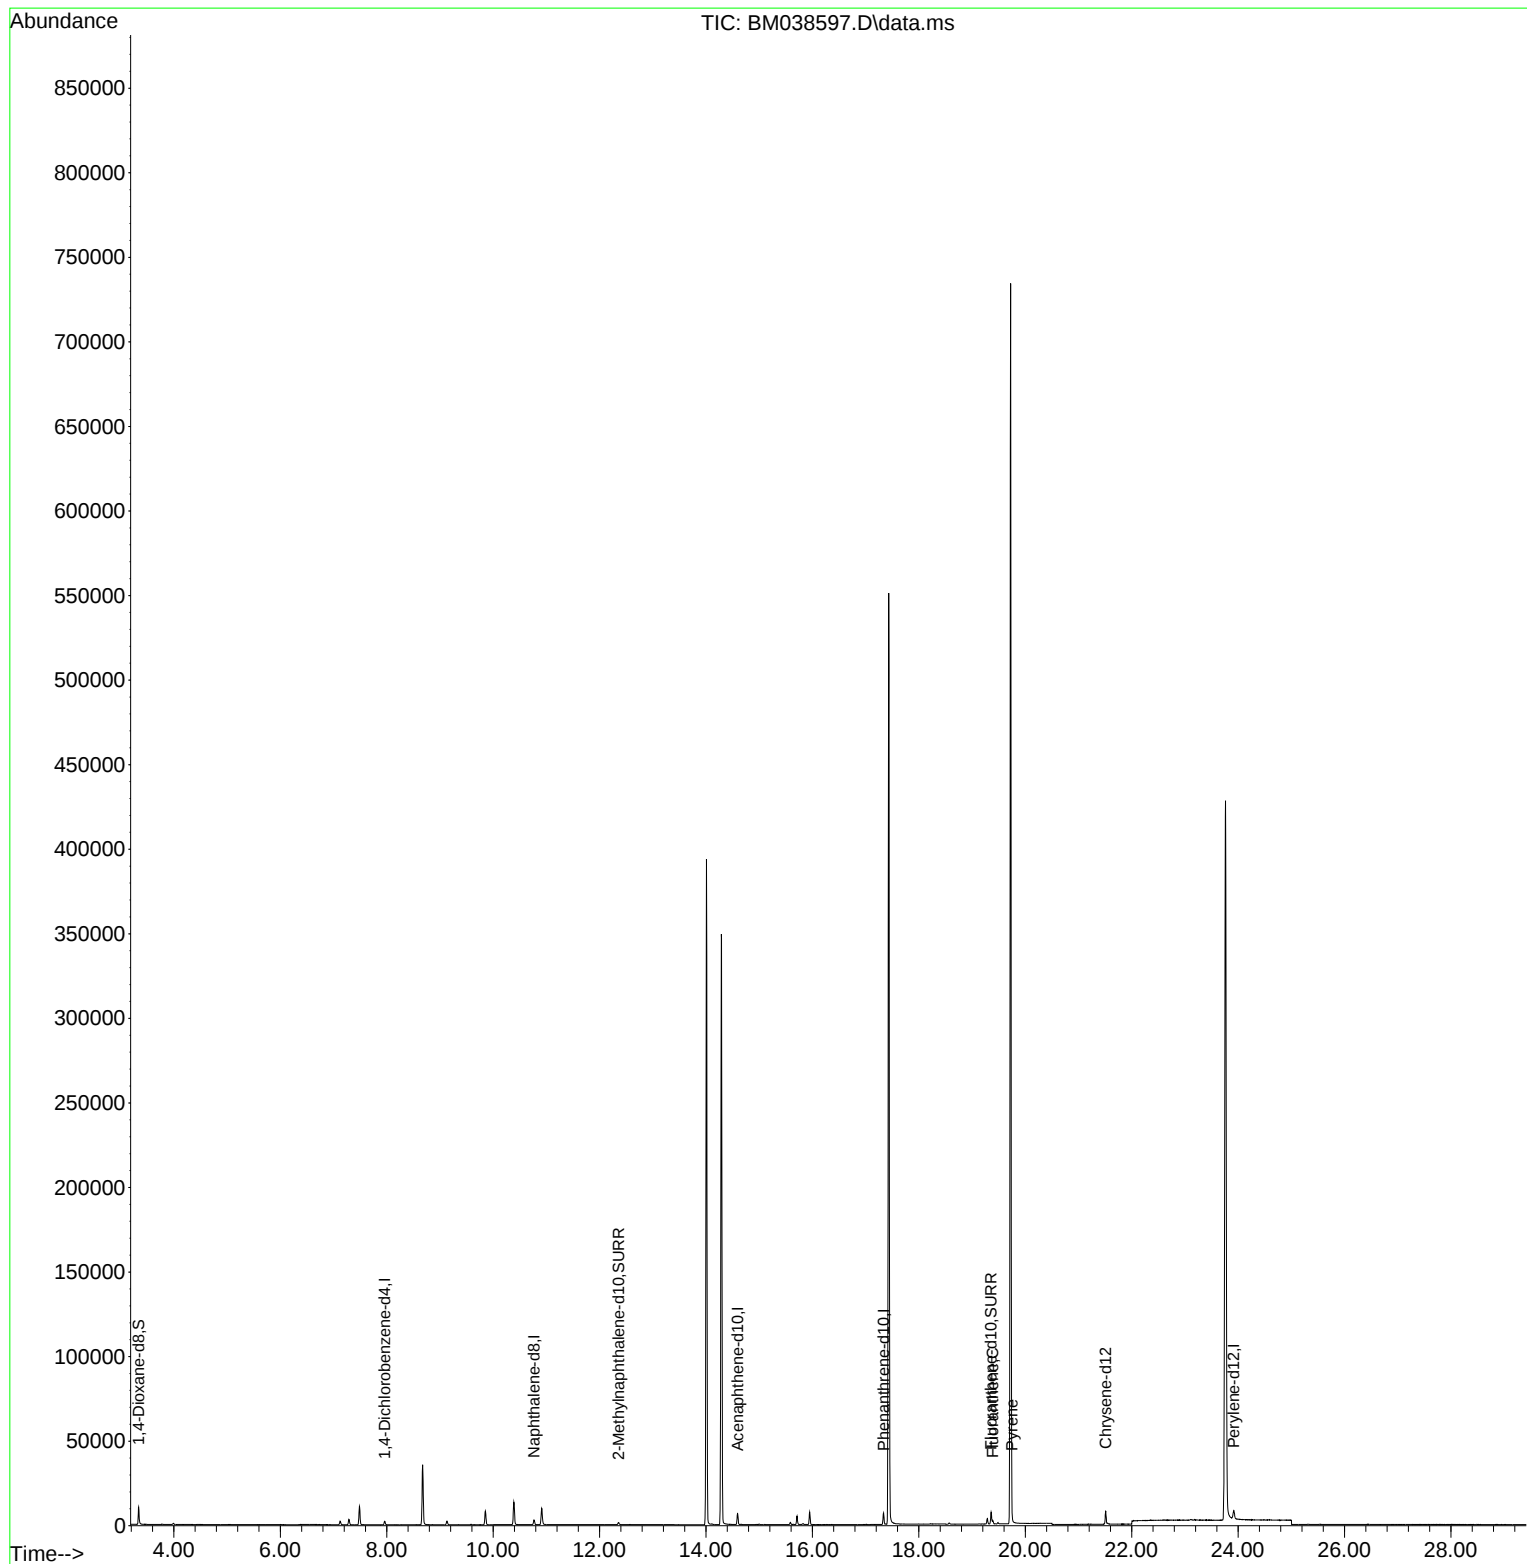


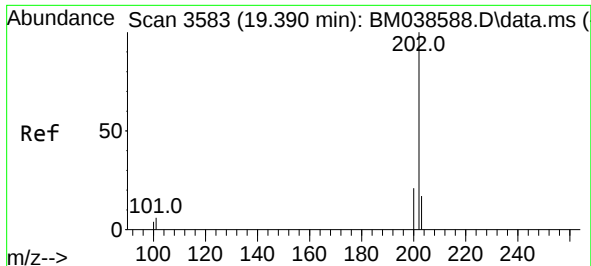

#19
Fluoranthene
Concen: 0.069 ng/ul
RT: 19.389 min Scan# 3583
Delta R.T. -0.005 min
Lab File: BM038597.D
Acq: 27 Jan 2023 22:26

Instrument :
BNA_M
ClientSampleId :
EX9G1

Tgt Ion:202 Resp: 1909
Ion Ratio Lower Upper
202 100
101 12.2 5.3 7.9#
100 9.2 4.2 6.2#

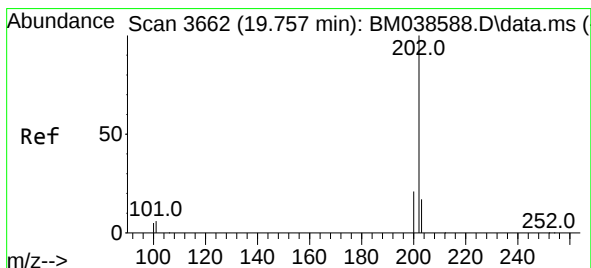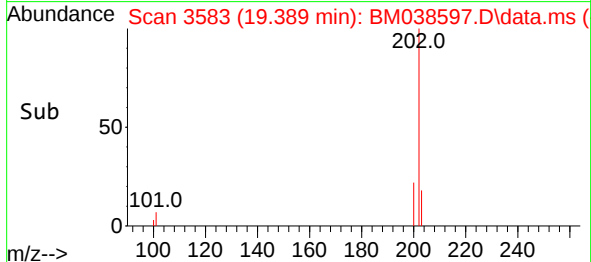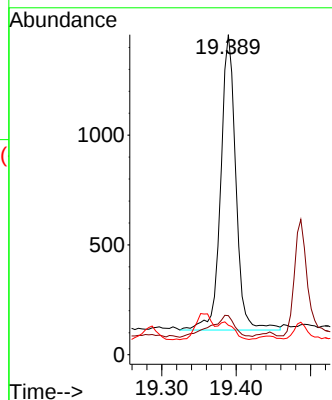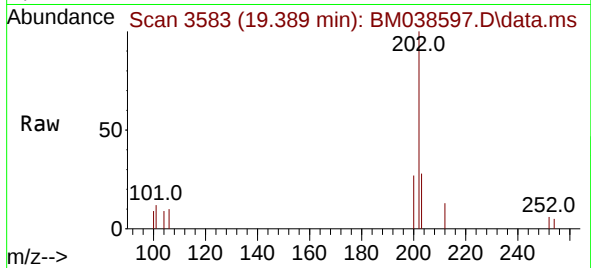

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.752 min Scan# 3661
Delta R.T. -0.005 min
Lab File: BM038597.D
Acq: 27 Jan 2023 22:26

Tgt Ion:202 Resp: 1478
Ion Ratio Lower Upper
202 100
101 13.6 5.9 8.9#
100 14.2 5.2 7.8#

