
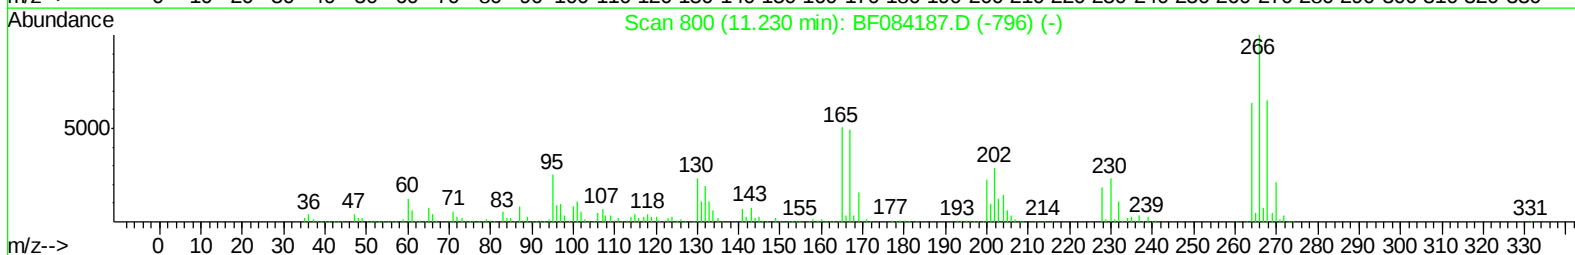
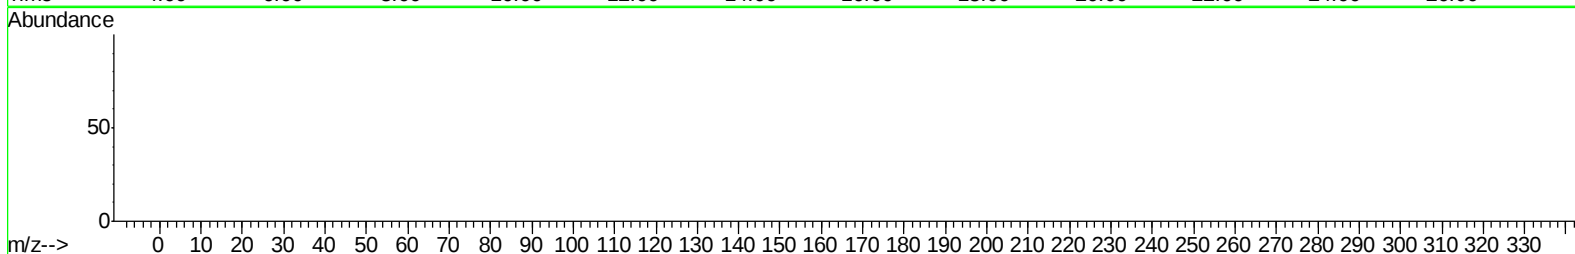


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012716\
Data File : BM004129.D
Acq On : 27 Jan 2016 10:27
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 07:54:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 16:24:07 2016
Response via : Initial Calibration

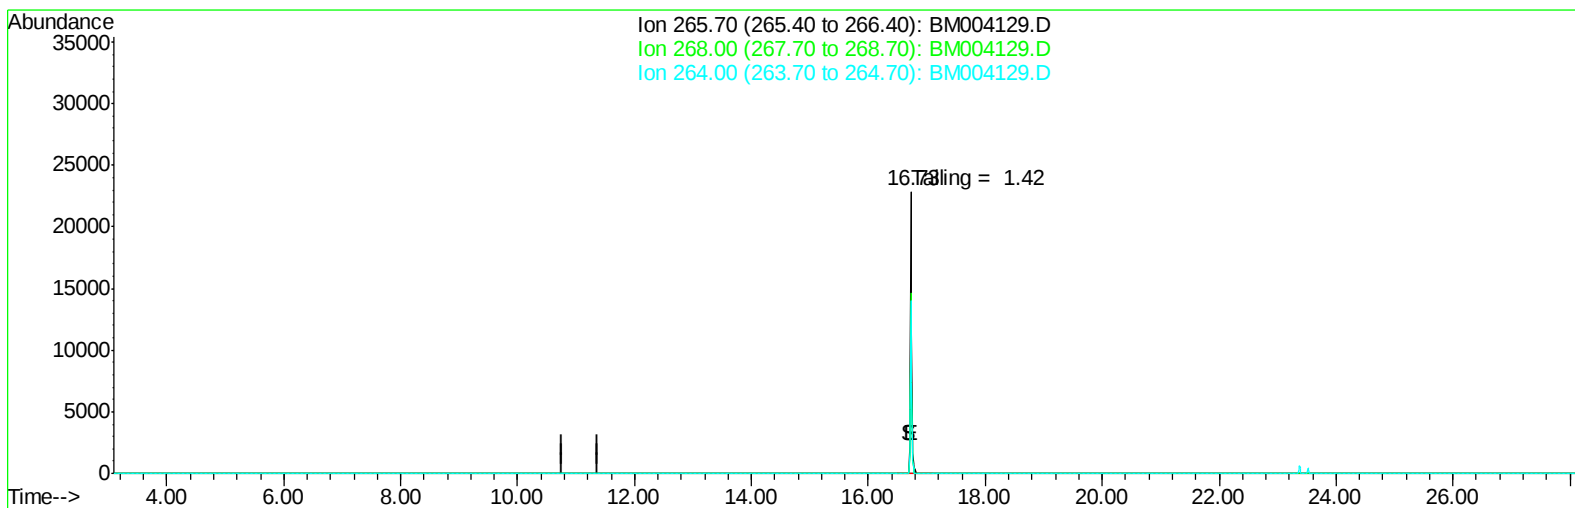

TIC: BM004129.D

(69) Pentachlorophenol (C)




11.070min (-11.070) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	65.50	0.00#
264.00	62.70	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012716\
Data File : BM004129.D
Acq On : 27 Jan 2016 10:27
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 07:54:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 16:24:07 2016
Response via : Initial Calibration

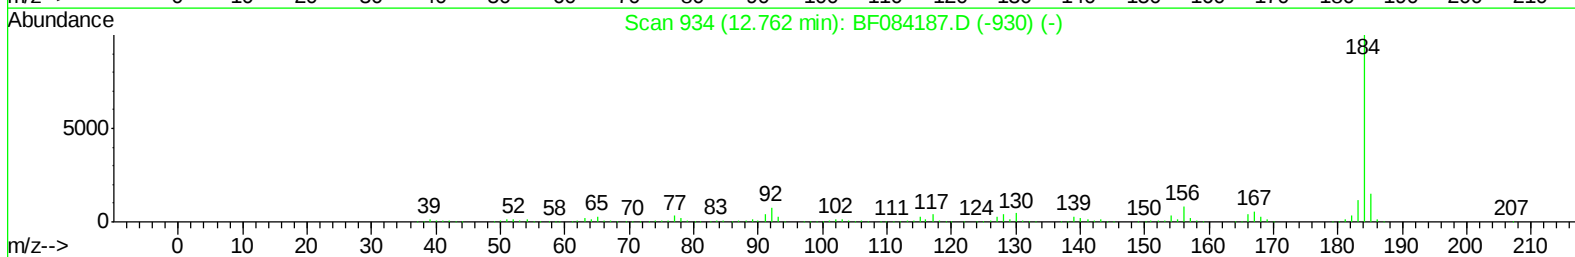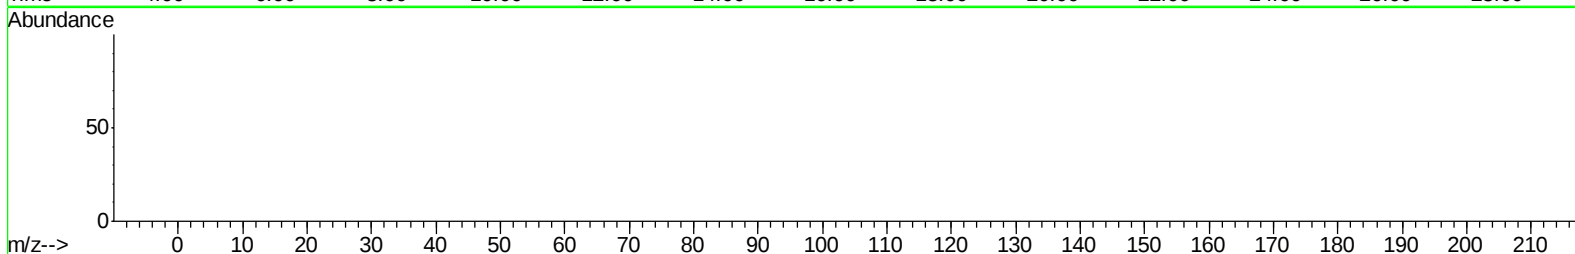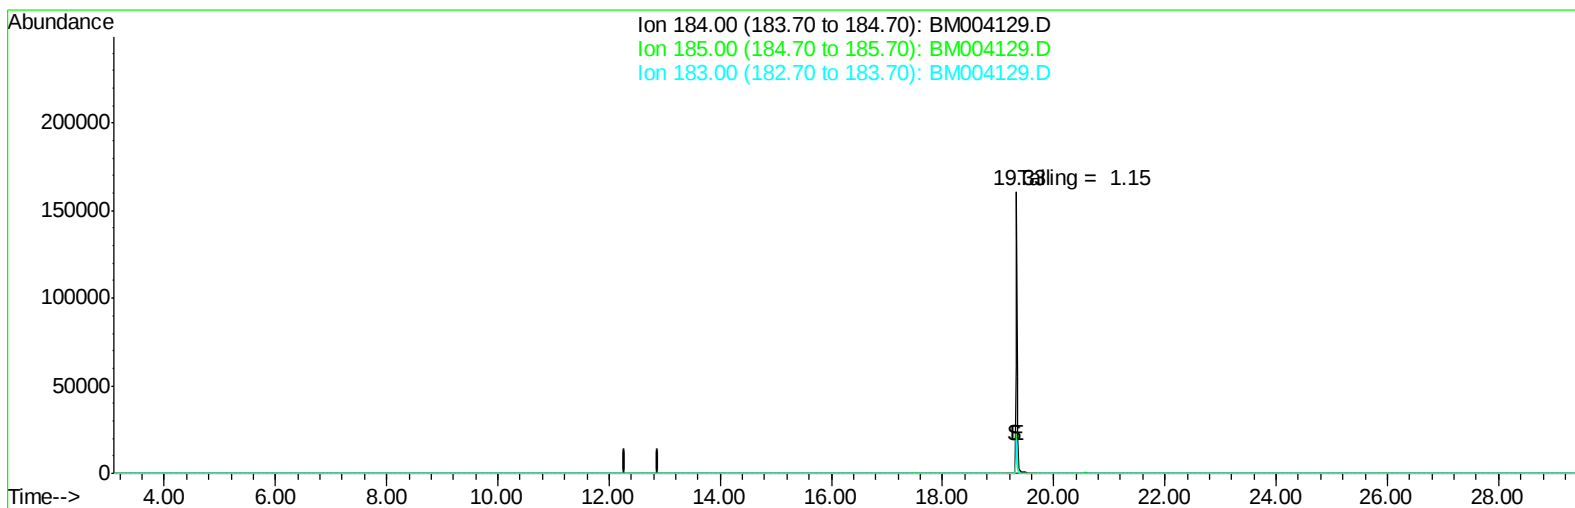

TIC: BM004129.D

(76) Benzidine

12.591min (-12.591) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.20	0.00#
183.00	12.30	0.00#
0.00	0.00	0.00