


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012716\
Data File : BM004129.D
Acq On : 27 Jan 2016 10:27
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM012216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 22 14:46:41 2016

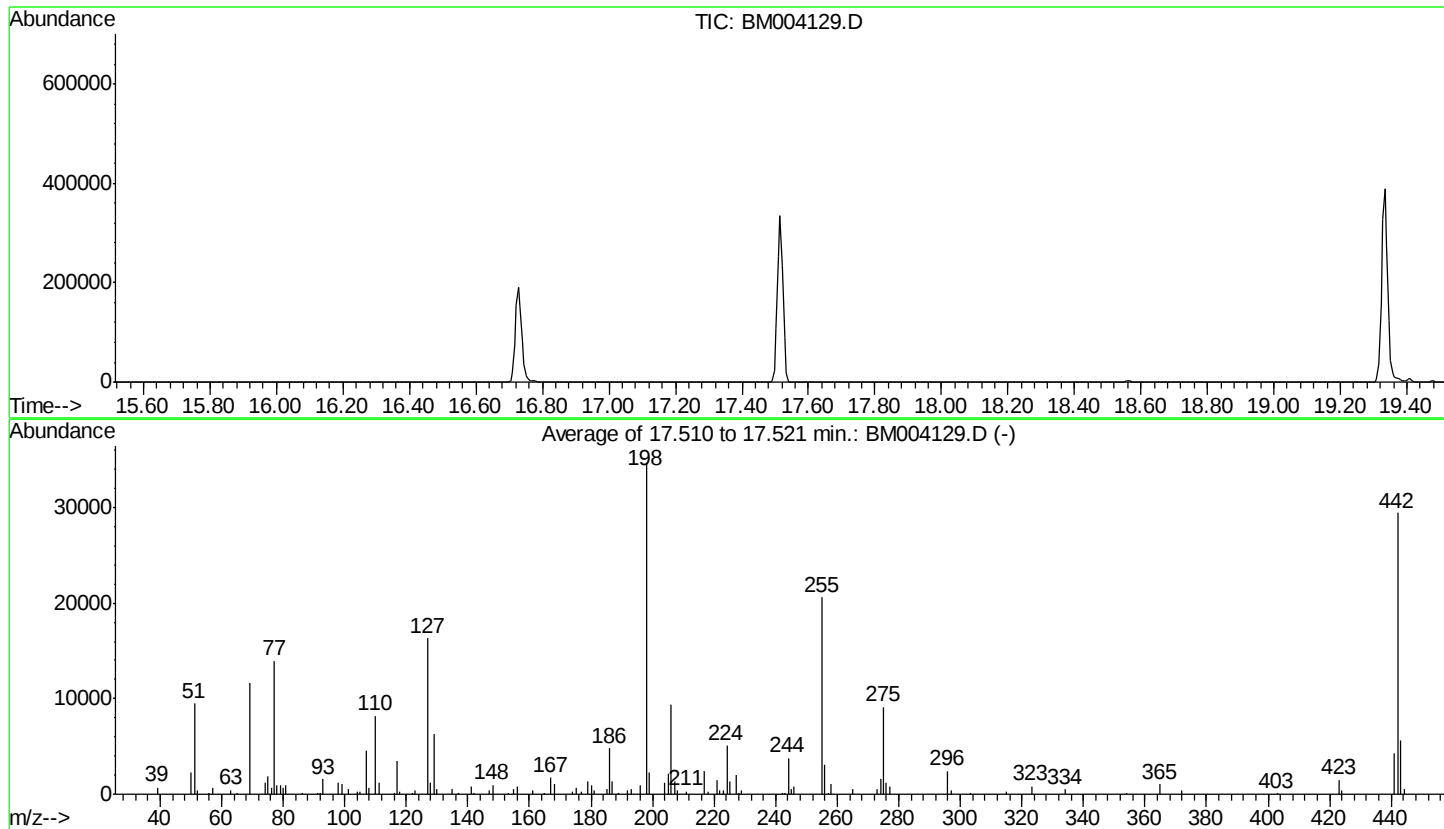

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	9503	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.7	11704	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	16300	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34685	PASS
199	198	5	9	6.7	2325	PASS
275	198	10	60	26.4	9174	PASS
365	198	1	100	3.0	1039	PASS
441	442	0.01	24	14.7	4314	PASS
442	198	50	100	84.9	29445	PASS
443	442	15	24	19.2	5668	PASS