

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012717\
 Data File : BM008915.D
 Acq On : 27 Jan 2017 23:26
 Operator : SJ/MA
 Sample : I1467-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDMX4

Quant Time: Jan 28 03:47:23 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 27 22:34:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	57704	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	225495	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	166936	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	352649	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	444991	20.00	ng/ul	0.00
83) Perylene-d12	23.83	264	437686	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.39	96	3170	2.72	ng/uL	0.00
5) Phenol-d5	7.07	99	49775	10.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	163142	41.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	108005	33.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	81139	21.20	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	63438	44.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.81	143	74095	42.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.34	165	138482	37.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	6284	1.58	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	490883	44.88	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	570232	44.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.75	143	15082	8.24	ng/ul	0.00
57) Fluorene-d10	15.56	176	430454	41.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	67131	31.97	ng/ul	0.00
70) Anthracene-d10	17.40	188	727667	47.18	ng/ul	0.00
76) Pyrene-d10	19.69	212	860994	44.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.68	264	810508	43.73	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
33) 4-Chloro-3-methylphenol	11.99	107	11982	2.57	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012717\
Data File : BM008915.D
Acq On : 27 Jan 2017 23:26
Operator : SJ/MA
Sample : I1467-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDMX4

Quant Time: Jan 28 03:47:23 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 27 22:34:22 2017
Response via : Initial Calibration

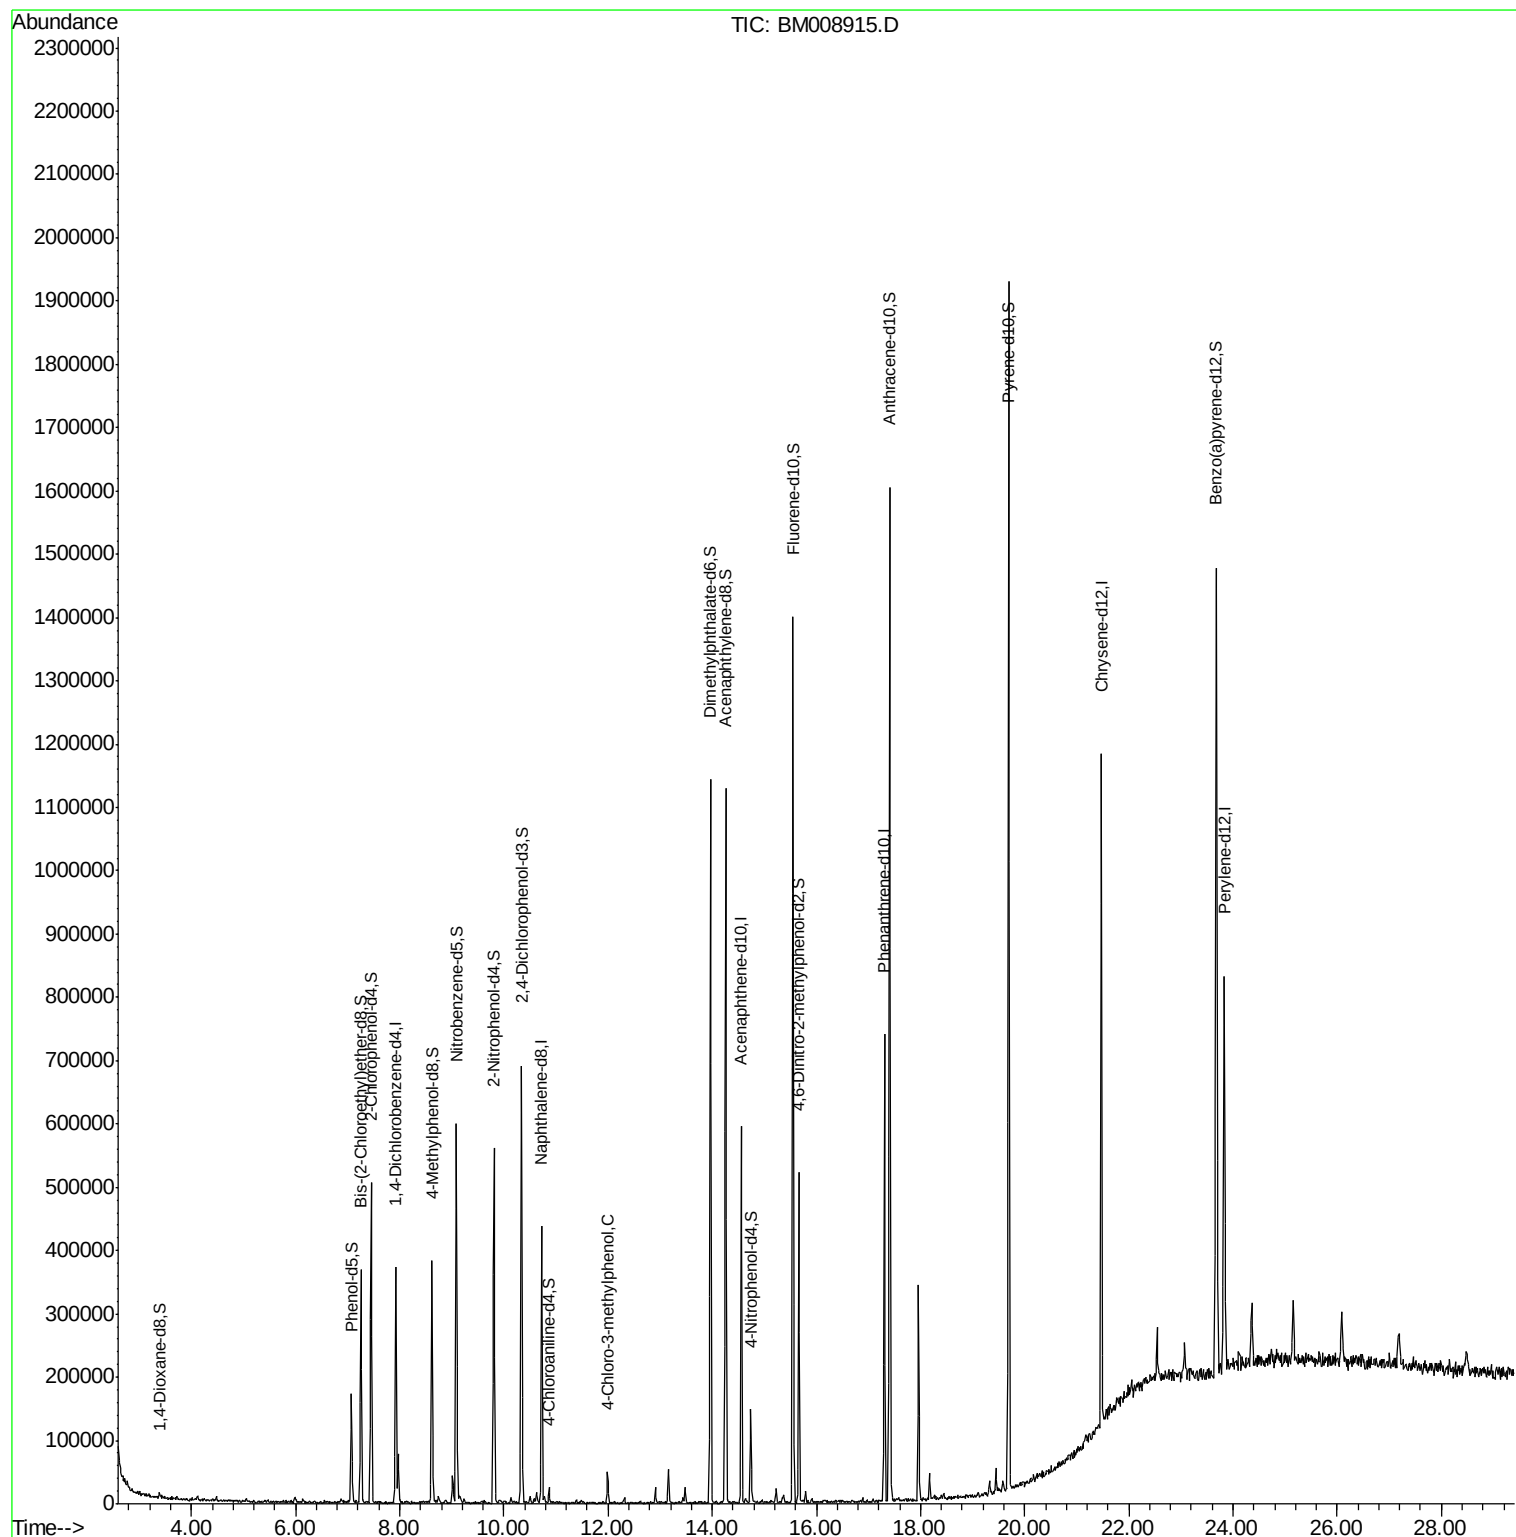

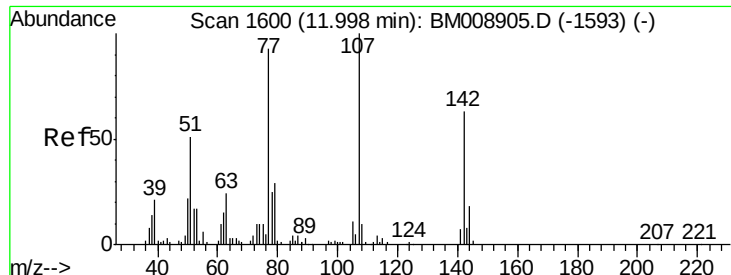

#33
 4-Chloro-3-methylphenol
 Concen: 2.57 ng/ul
 RT: 11.99 min Scan# 1599
 Delta R.T. -0.01 min
 Lab File: BM008915.D
 Acq: 27 Jan 2017 23:26

Instrument :
 BNA_M
 ClientSampleId :
 BDMX4

Tgt Ion	Ratio	Lower	Upper
107	100		
144	28.7	19.4	29.2
142	68.9	58.0	87.0

