

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012717\
 Data File : BM008906.D
 Acq On : 27 Jan 2017 17:37
 Operator : SJ/MA
 Sample : PB96397BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	132	135	142	rVB2	38943	53062	1.97%	0.146%
2	7.075	756	763	772	rVB	736683	1115079	41.44%	3.058%
3	7.257	785	794	801	rBV	449657	698506	25.96%	1.916%
4	7.457	821	828	834	rBV	694263	1094446	40.67%	3.001%
5	7.928	899	908	916	rBV	478171	770964	28.65%	2.114%
6	8.622	1015	1026	1033	rBV	758455	1242430	46.17%	3.407%
7	9.092	1099	1106	1113	rBV	687760	1151418	42.79%	3.158%
8	9.810	1221	1228	1236	rVB	593914	992117	36.87%	2.721%
9	10.339	1310	1318	1327	rBV	792783	1315271	48.88%	3.607%
10	10.728	1376	1384	1394	rVB	568487	957801	35.60%	2.627%
11	10.863	1400	1407	1416	rVB	677838	1153137	42.86%	3.162%
12	13.969	1928	1935	1941	rBV	1328308	1764205	65.57%	4.838%
13	14.257	1975	1984	1993	rBV	1248145	1838855	68.34%	5.043%
14	14.563	2030	2036	2042	rBV	821308	1168326	43.42%	3.204%
15	14.745	2060	2067	2077	rBV	728429	1013582	37.67%	2.780%
16	15.557	2198	2205	2212	rVB	1586015	2225598	82.71%	6.104%
17	15.668	2218	2224	2235	rVB	567307	735420	27.33%	2.017%
18	17.309	2495	2503	2510	rBV	957162	1316589	48.93%	3.611%
19	17.409	2513	2520	2527	rVV	1661651	2383695	88.59%	6.537%
20	19.486	2863	2873	2883	rBV	738379	1544277	57.39%	4.235%
21	19.698	2903	2909	2915	rBV	1912616	2596281	96.49%	7.120%
22	21.474	3206	3211	3218	rBV	1105350	1471182	54.68%	4.035%
23	22.674	3408	3415	3424	rVB2	1358372	2690755	100.00%	7.379%
24	22.850	3438	3445	3453	rBV2	673756	1401495	52.09%	3.844%
25	23.686	3580	3587	3594	rBV2	1264213	2447619	90.96%	6.713%
26	23.838	3607	3613	3622	rVB	640067	1321435	49.11%	3.624%


Sum of corrected areas: 36463545

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012717\
Data File : BM008906.D
Acq On : 27 Jan 2017 17:37
Operator : SJ/MA
Sample : PB96397BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK97

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

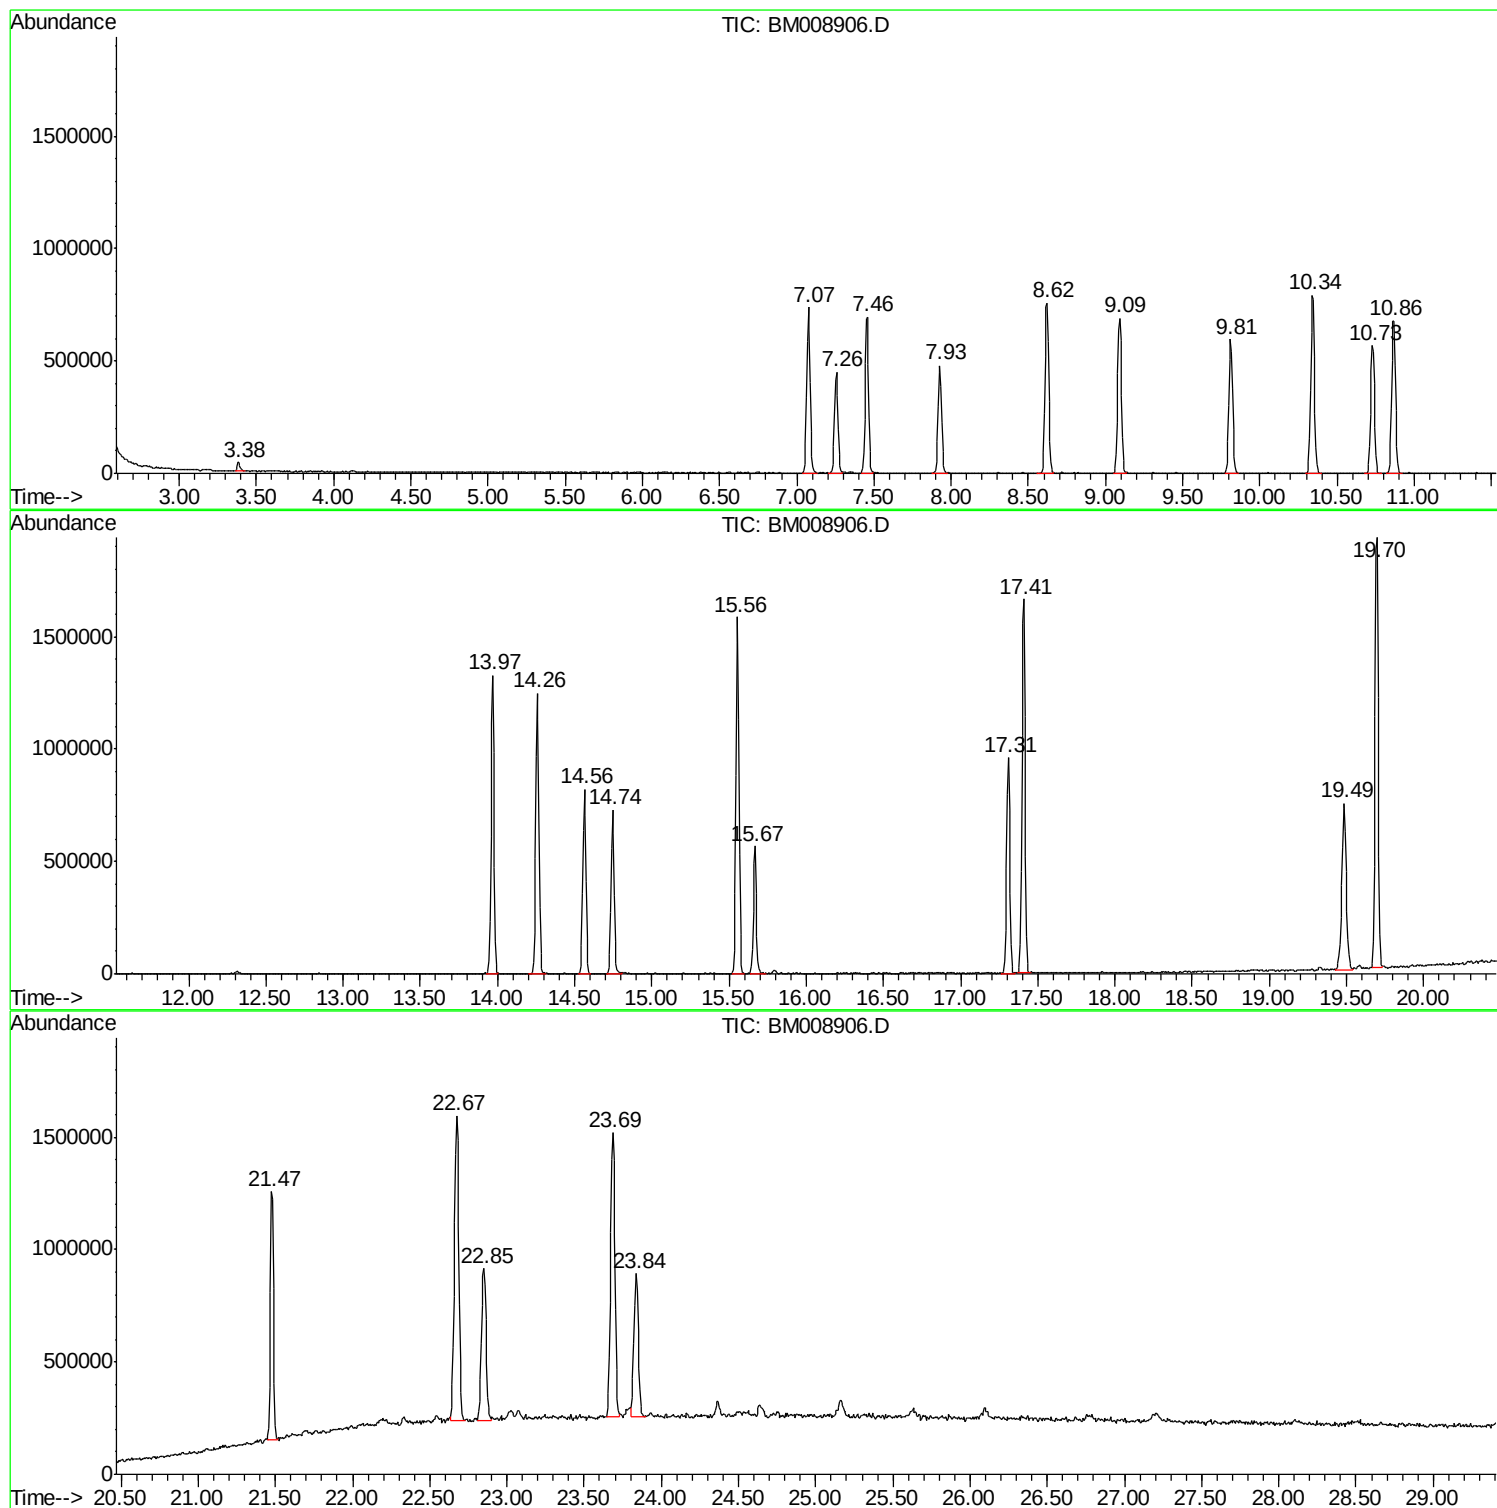

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012717\
Data File : BM008906.D
Acq On : 27 Jan 2017 17:37
Operator : SJ/MA
Sample : PB96397BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK97

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012717\
Data File : BM008906.D
Acq On : 27 Jan 2017 17:37
Operator : SJ/MA
Sample : PB96397BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK97

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc