

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012718\
 Data File : BM013889.D
 Acq On : 27 Jan 2018 18:07
 Operator : SJ/JU
 Sample : J1244-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6B57

Quant Time: Jan 28 01:06:27 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jan 28 01:01:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	128826	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	495138	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	284236	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	633812	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	665291	20.00	ng/ul	0.00
83) Perylene-d12	23.38	264	680976	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	13228	4.06	ng/uL	0.00
5) Phenol-d5	6.77	99	264018	26.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	166421	27.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	230605	28.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	219245	28.84	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	112131	29.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	119911	29.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	224518	28.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	276067	40.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	725193	30.96	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	905889	30.32	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	70522	18.52	ng/ul	0.00
57) Fluorene-d10	15.23	176	617535	29.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	78848	20.67	ng/ul	0.00
70) Anthracene-d10	16.99	188	633812	20.53	ng/ul	-0.09
76) Pyrene-d10	19.39	212	1041107	33.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	1009752	32.26	ng/ul	0.00
Target Compounds						
6) Phenol	6.79	94	36001	3.629	ng/ul	92
44) Dimethylphthalate	13.70	163	150327	6.527	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012718\
Data File : BM013889.D
Acq On : 27 Jan 2018 18:07
Operator : SJ/JU
Sample : J1244-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6B57

Quant Time: Jan 28 01:06:27 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jan 28 01:01:50 2018
Response via : Initial Calibration

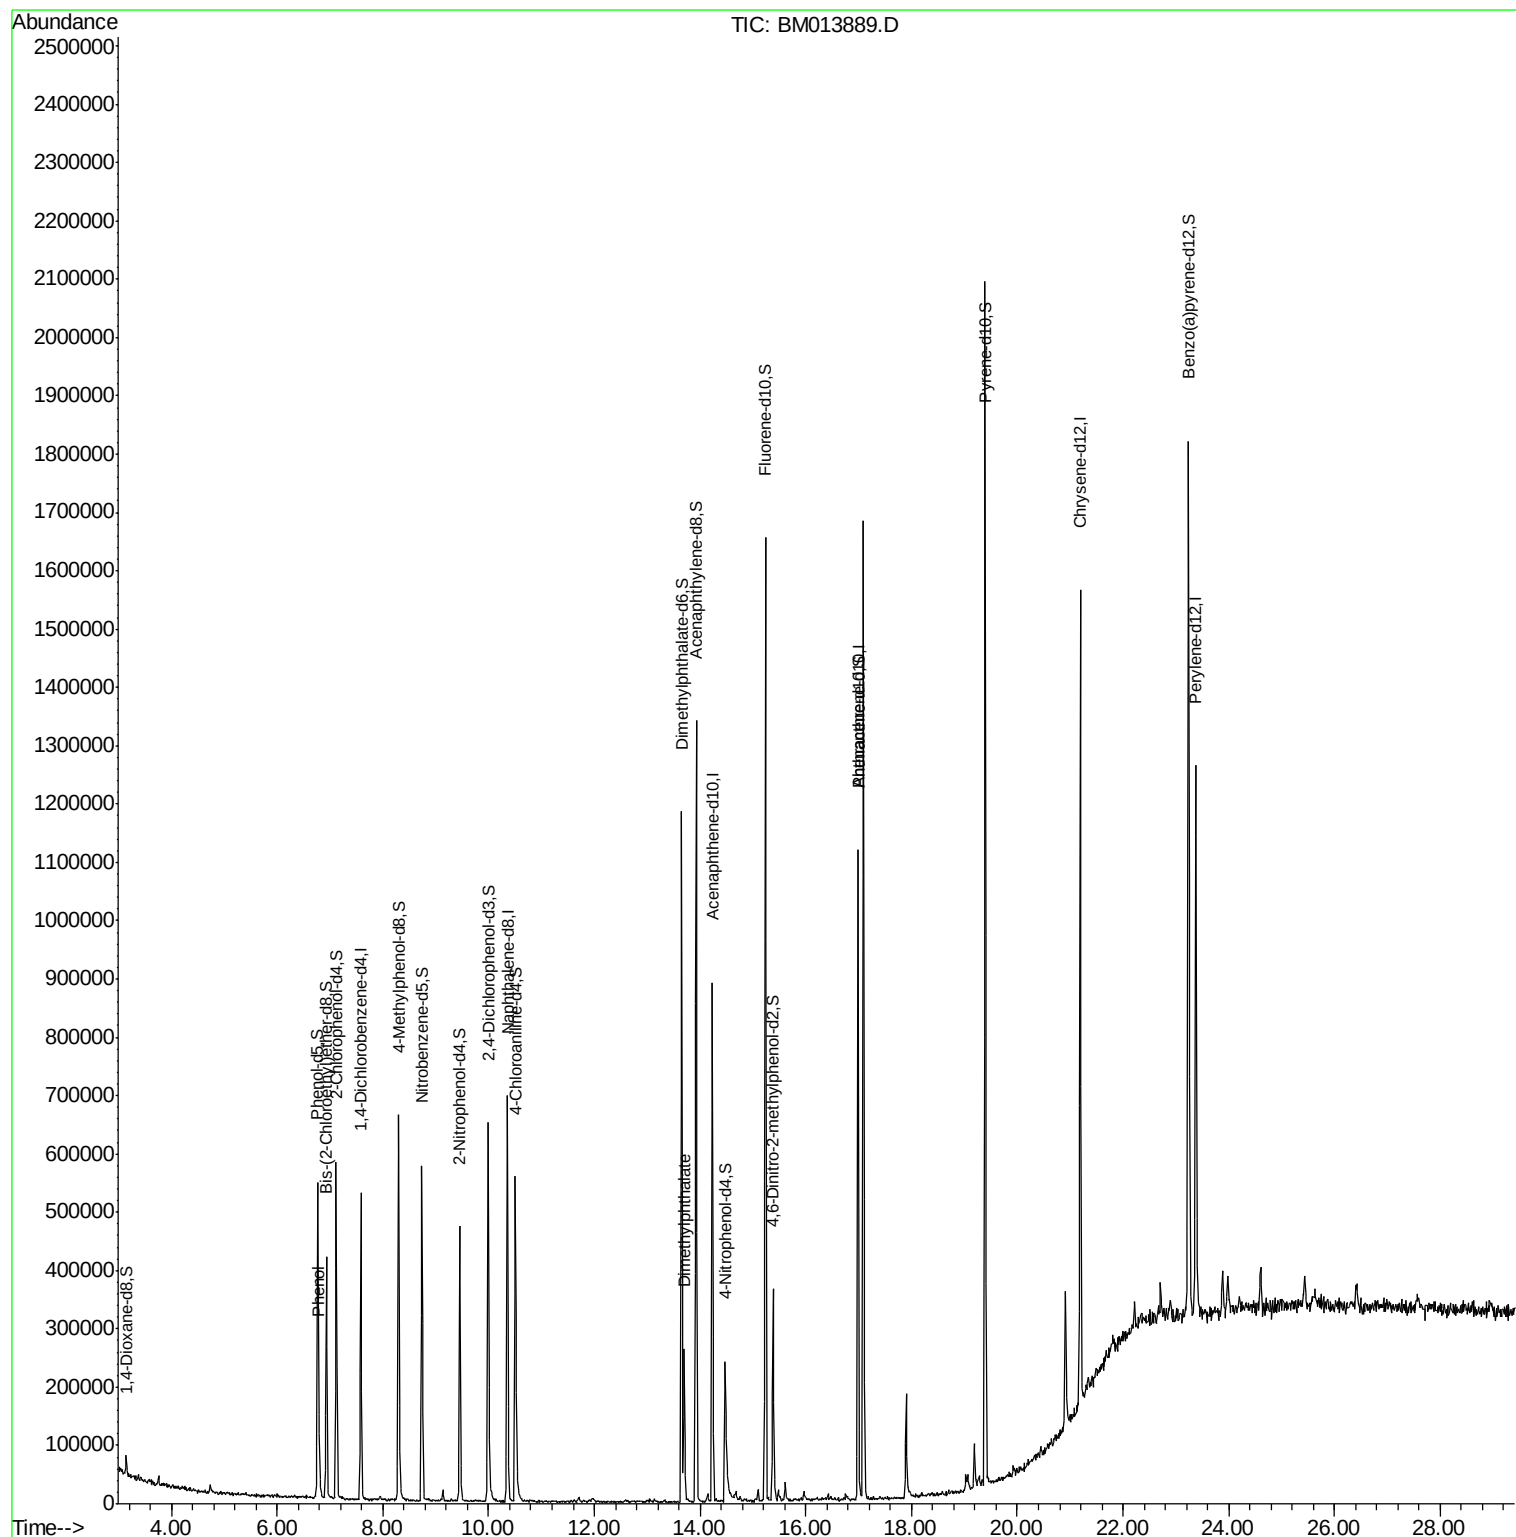

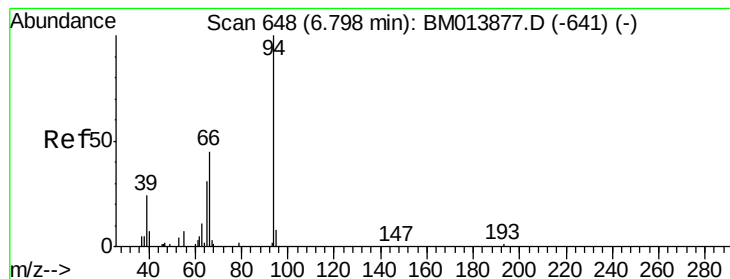





#6

Phenol

Concen: 3.629 ng/ul
 RT: 6.79 min Scan# 647
 Delta R.T. -0.01 min
 Lab File: BM013889.D
 Acq: 27 Jan 2018 18:07

Instrument :
 BNA_M
 ClientSampled :
 F6B57

Tot Ion: 94 Resp: 36001
 Ion Ratio Lower Upper
 94 100
 65 35.1 28.2 42.4
 66 49.9 47.2 70.8

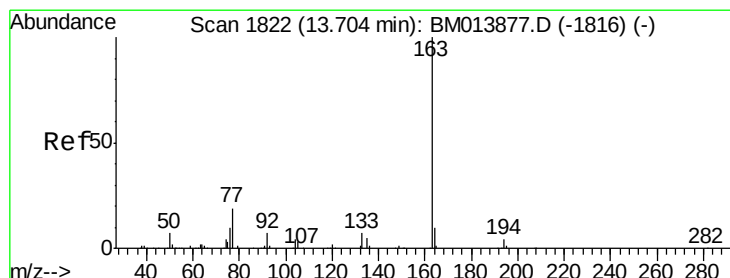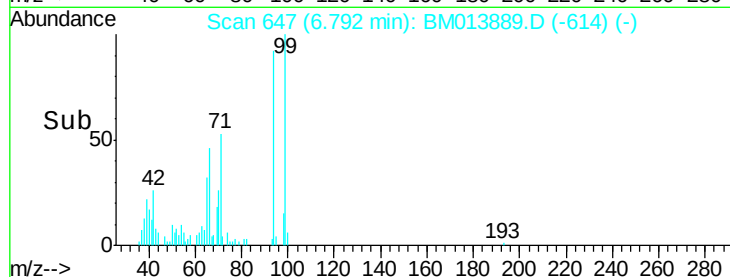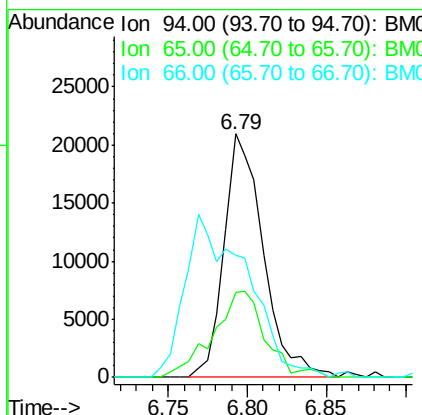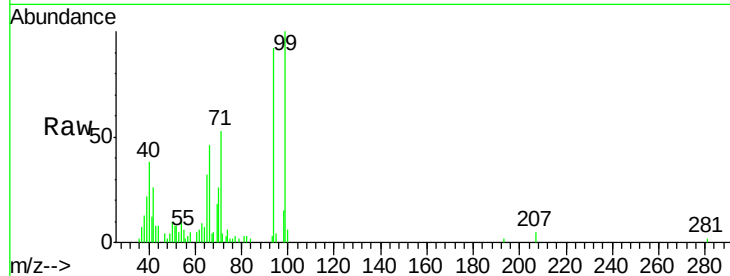

#44

Dimethylphthalate

Concen: 6.527 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.00 min
 Lab File: BM013889.D
 Acq: 27 Jan 2018 18:07

Tgt Ion: 163 Resp: 150327
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.5 5.3
 164 11.9 8.2 12.4

