

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012718\
 Data File : BM013898.D
 Acq On : 27 Jan 2018 23:30
 Operator : SJ/JU
 Sample : J1282-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6B85

Quant Time: Jan 28 02:50:10 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jan 28 02:49:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	136521	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	545779	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	332042	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	768602	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	743361	20.00	ng/ul	0.00
83) Perylene-d12	23.38	264	702574	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	18244	5.28	ng/uL	0.00
5) Phenol-d5	6.77	99	353575	33.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	227682	35.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	307906	36.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	320051	39.72	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	163047	38.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	178380	39.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	330523	38.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	418417	55.79	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	1084014	39.61	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	1386304	39.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	111079	24.98	ng/ul	0.00
57) Fluorene-d10	15.23	176	937600	38.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	132991	28.75	ng/ul	0.00
70) Anthracene-d10	17.09	188	1415556	37.81	ng/ul	0.00
76) Pyrene-d10	19.39	212	1551666	44.83	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.38	264	692869	21.46	ng/ul	0.14

Target Compounds


				Ovalue	
6) Phenol	6.79	94	60804	5.784	ng/ul 95
15) N-Nitroso-di-n-propylamine	8.29	70	10457	1.608	ng/ul# 1
21) Isophorone	9.46	82	20367	1.152	ng/ul# 77
44) Dimethylphthalate	13.70	163	162813	6.051	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012718\
Data File : BM013898.D
Acq On : 27 Jan 2018 23:30
Operator : SJ/JU
Sample : J1282-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6B85

Quant Time: Jan 28 02:50:10 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jan 28 02:49:11 2018
Response via : Initial Calibration

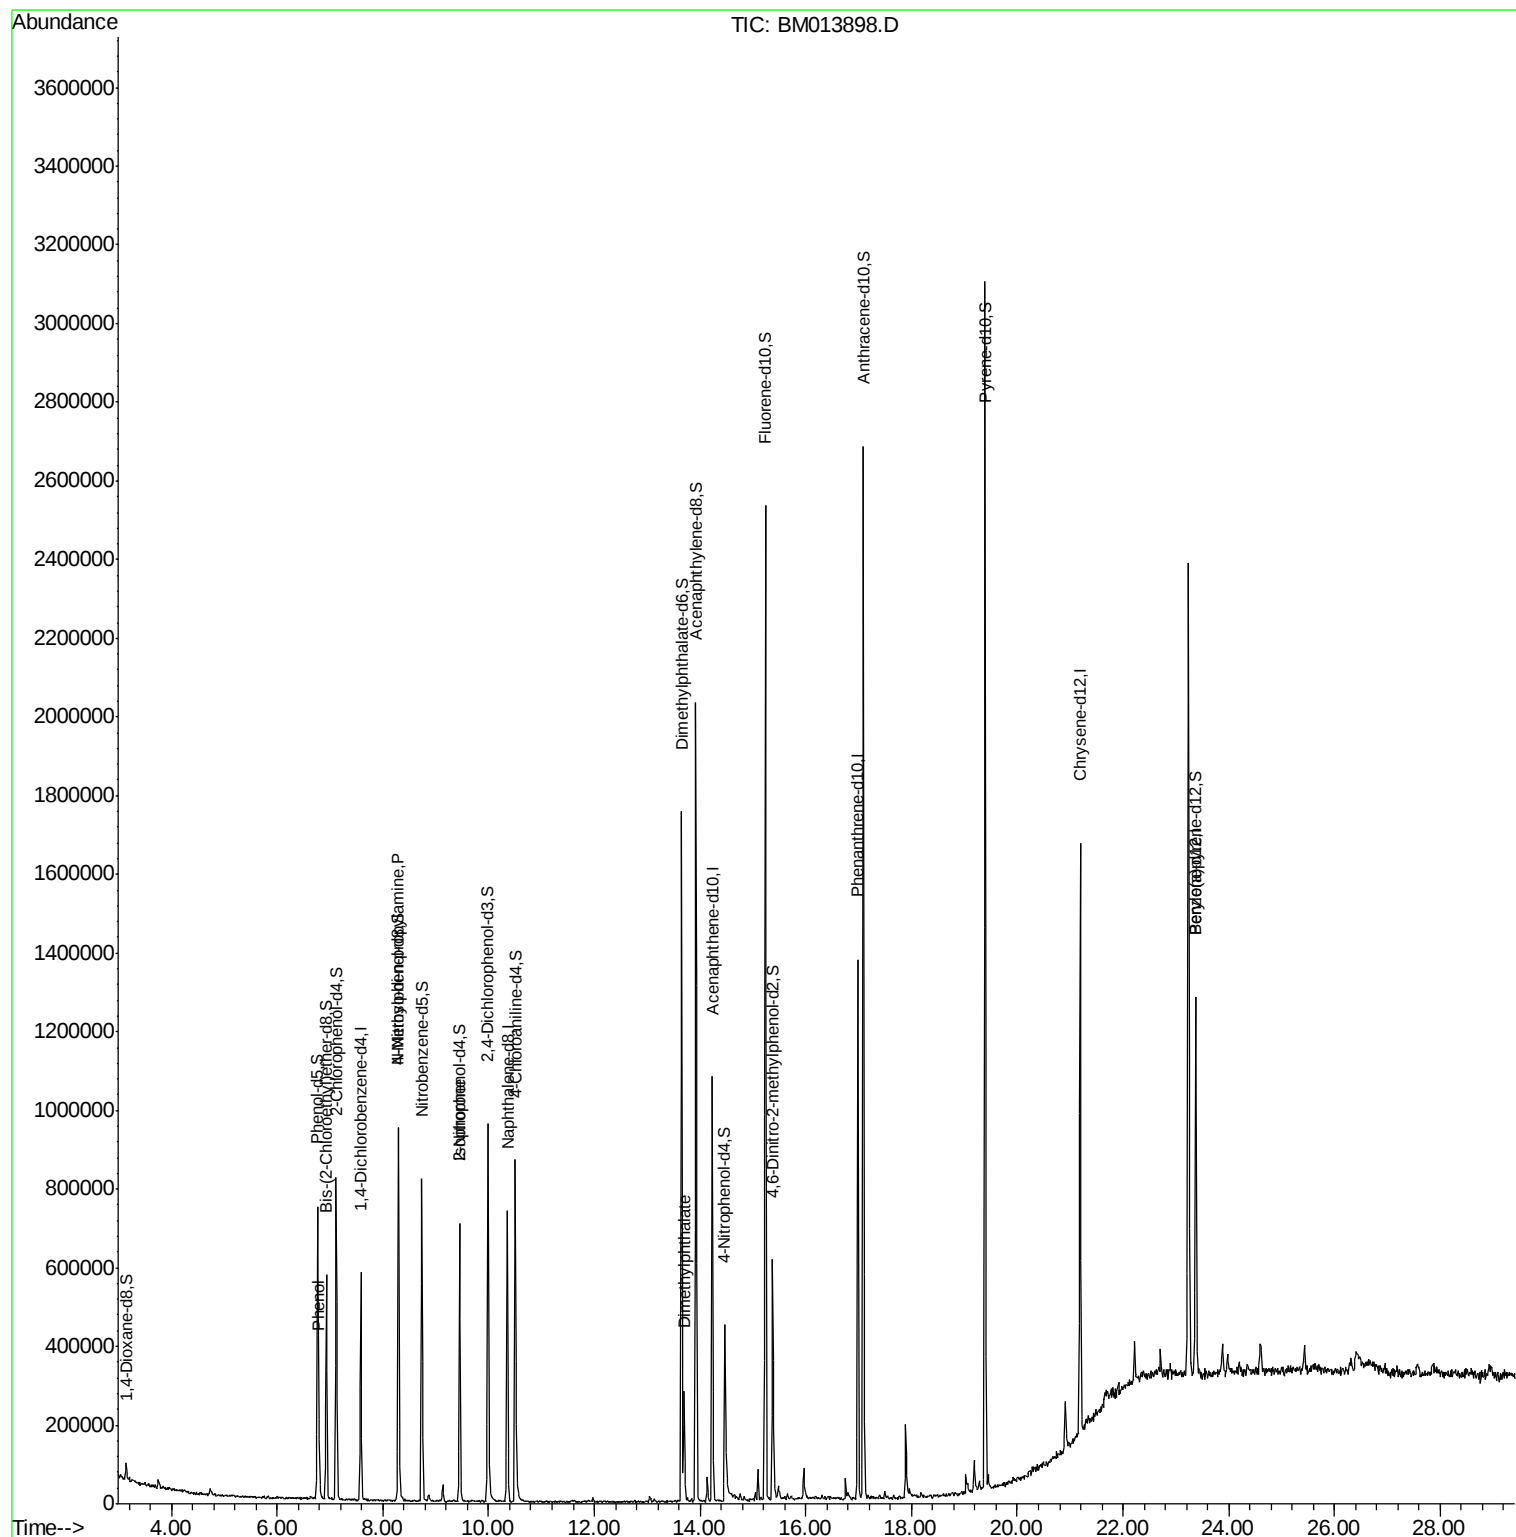

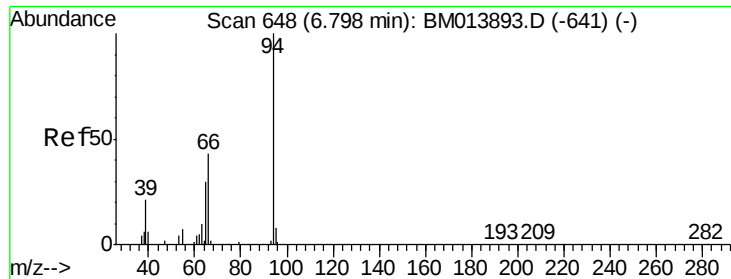





#6

Phenol

Concen: 5.784 ng/ul
 RT: 6.79 min Scan# 647
 Delta R.T. -0.01 min
 Lab File: BM013898.D
 Acq: 27 Jan 2018 23:30

Instrument :
 BNA_M
 ClientSampleId :
 F6B85

Tot Ion	94	Resp	60804
Ion Ratio	100	Lower	Upper
94	100		
65	35.5	28.2	42.4
66	53.4	47.2	70.8

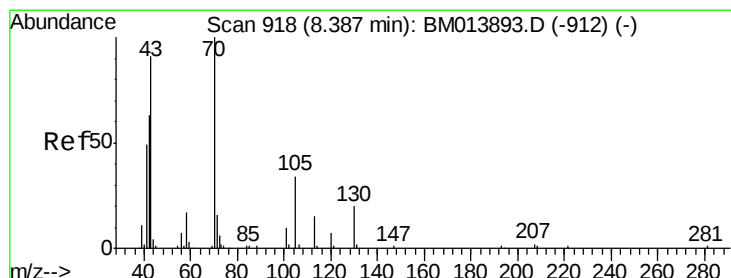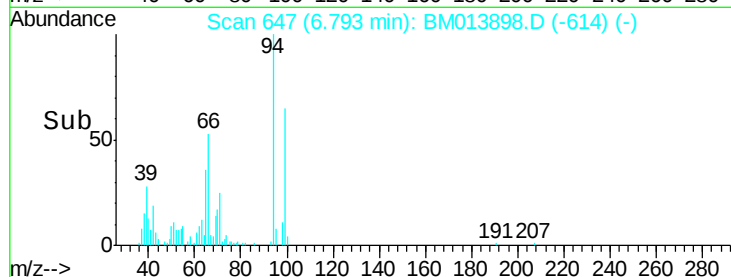
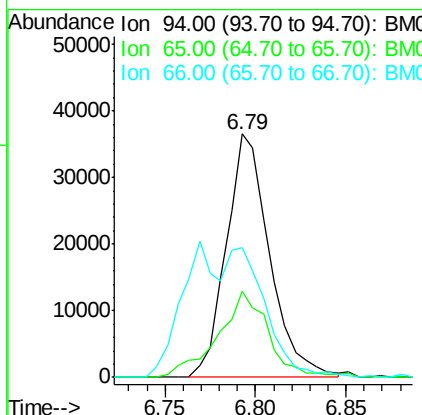
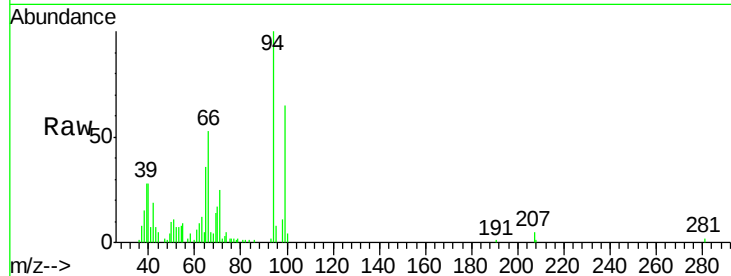



#15

N-Nitroso-di-n-propylamine

Concen: 1.608 ng/ul
 RT: 8.29 min Scan# 902
 Delta R.T. -0.09 min
 Lab File: BM013898.D
 Acq: 27 Jan 2018 23:30

Tgt Ion	70	Resp	10457
Ion Ratio	100	Lower	Upper
70	100		
42	446.7	76.0	114.0#
101	0.0	6.7	10.1#
130	0.0	14.6	22.0#

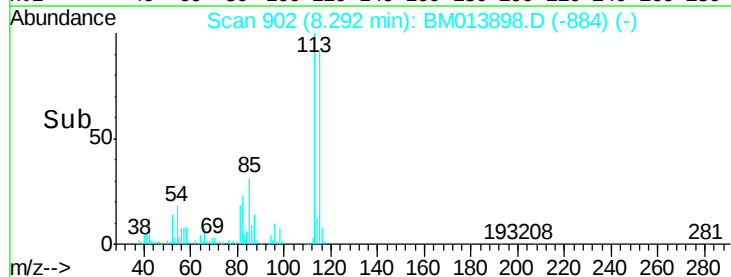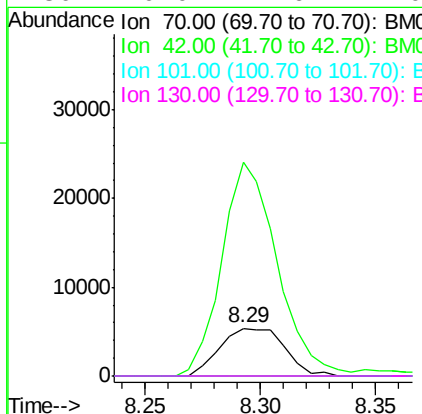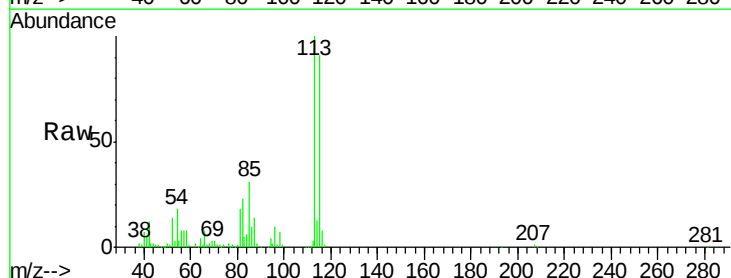

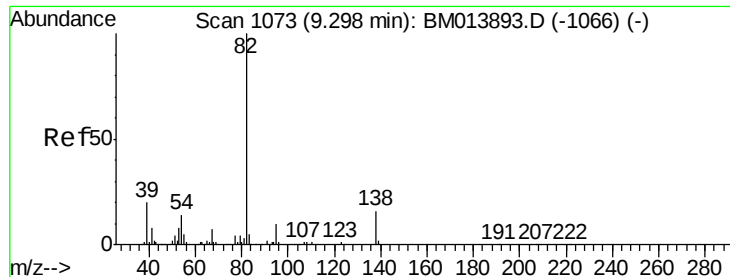

#21

Isophorone

Concen: 1.152 ng/ul

RT: 9.46 min Scan# 1100

Delta R.T. 0.16 min

Lab File: BM013898.D

Acq: 27 Jan 2018 23:30

Instrument :

BNA_M

ClientSampleId :

F6B85


Tot Ion: 82 Resp: 20367

Ion Ratio Lower Upper

82 100

95 11.5 7.8 11.8

138 0.0 11.9 17.9#


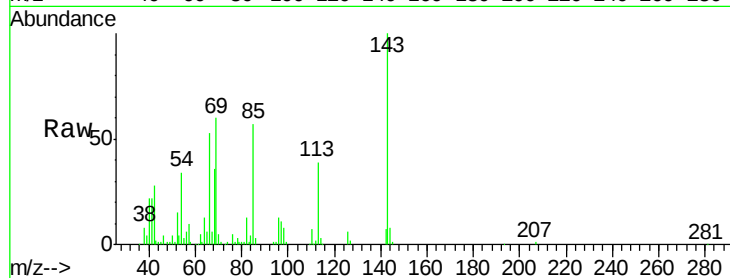


Abundance Ion 82.00 (81.70 to 82.70): BM013898.D (-1039) (-)

Ion 95.00 (94.70 to 95.70): BM013898.D (-1039) (-)

Ion 138.00 (137.70 to 138.70): BM013898.D (-1039) (-)

Time-->

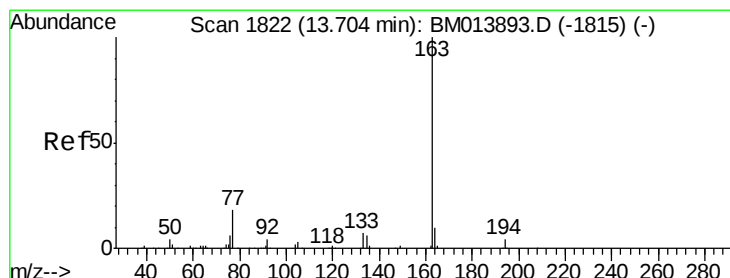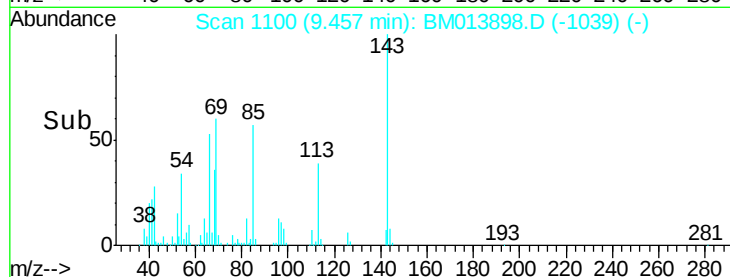

#44

Dimethylphthalate

Concen: 6.051 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.00 min

Lab File: BM013898.D

Acq: 27 Jan 2018 23:30


Tgt Ion: 163 Resp: 162813

Ion Ratio Lower Upper

163 100

194 4.8 3.5 5.3

164 10.1 8.2 12.4

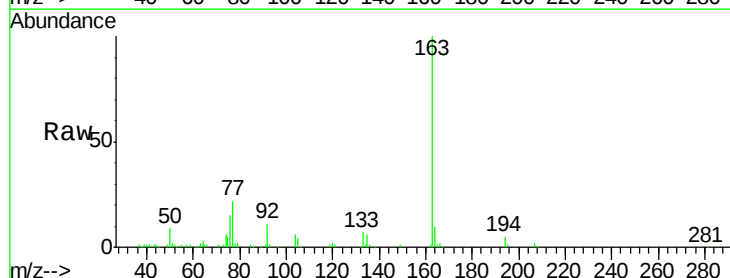

Abundance Ion 163.00 (162.70 to 163.70): BM013898.D (-1788) (-)

Ion 194.00 (193.70 to 194.70): BM013898.D (-1788) (-)

Ion 164.00 (163.70 to 164.70): BM013898.D (-1788) (-)

Time-->

