

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012718\
 Data File : BM013902.D
 Acq On : 28 Jan 2018 01:53
 Operator : SJ/JU
 Sample : J1282-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6B95

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:04:32 PM

Quant Time: Jan 28 03:13:34 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jan 28 02:49:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	129067	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	498106	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	299023	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	686443	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	685905	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	667573	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	14751	4.52	ng/uL	0.00
5) Phenol-d5	6.77	99	302603	30.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	191568	31.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	259869	32.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	248724	32.65	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	136679	35.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	151966	37.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	267644	33.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	343347	50.16	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	910120	36.93	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1141316	36.31	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	97249	24.28	ng/ul	0.00
57) Fluorene-d10	15.23	176	794606	36.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	109010	26.38	ng/ul	0.00
70) Anthracene-d10	17.09	188	1227421m	36.71	ng/ul	0.00
76) Pyrene-d10	19.39	212	1337368	41.88	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	1226751	39.98	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	87881	3.627	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012718\
Data File : BM013902.D
Acq On : 28 Jan 2018 01:53
Operator : SJ/JU
Sample : J1282-17
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6B95

Manual Integrations
APPROVED

Sohil
1/29/2018 6:04:32 PM

Quant Time: Jan 28 03:13:34 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jan 28 02:49:11 2018
Response via : Initial Calibration

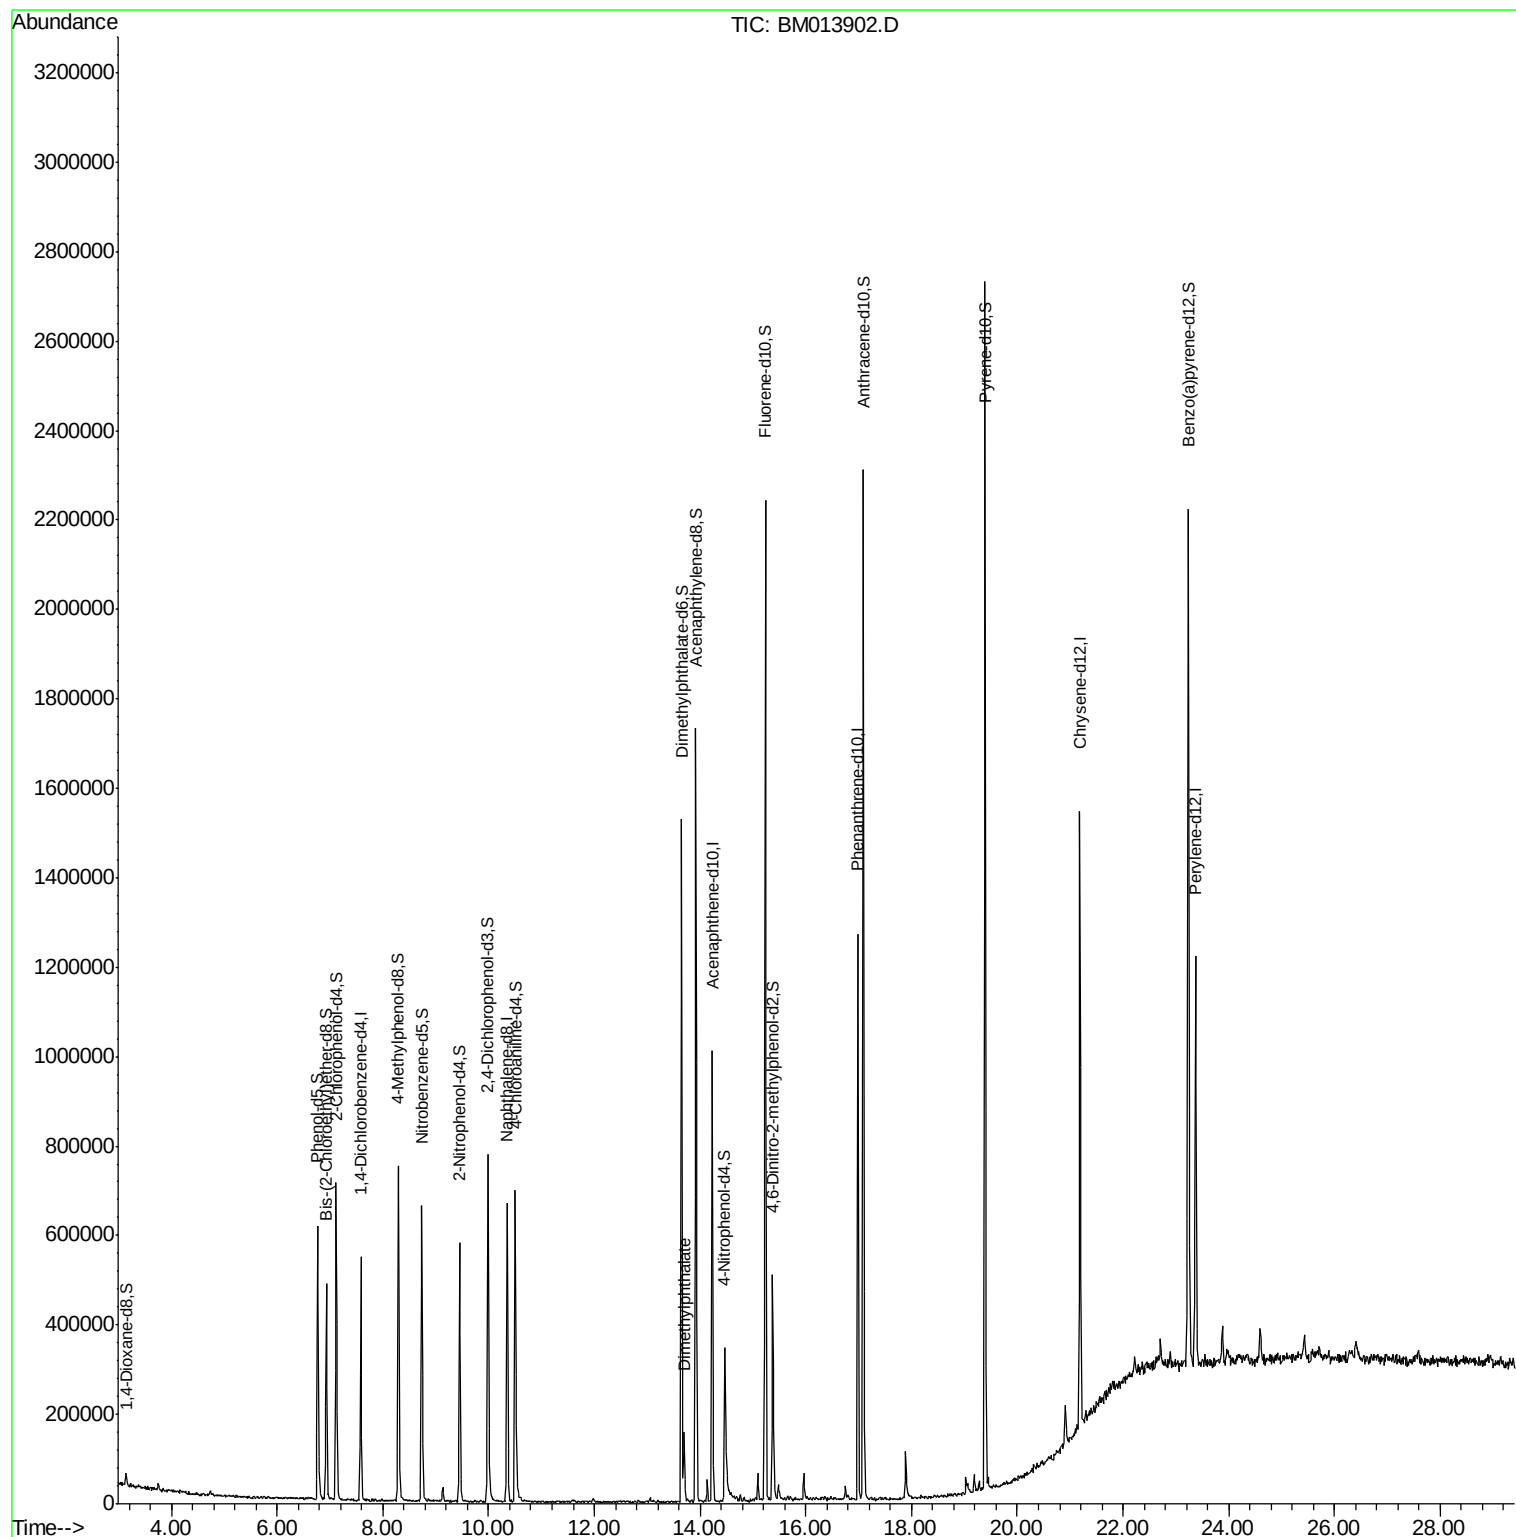

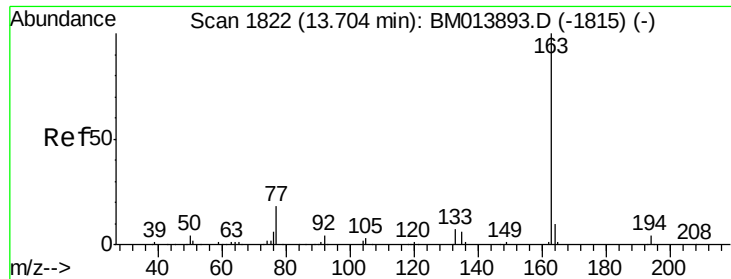

#44
 Dimethylphthalate
 Concen: 3.627 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.00 min
 Lab File: BM013902.D
 Acq: 28 Jan 2018 01:53

Instrument :
 BNA_M
 ClientSampleId :
 F6B95

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	3.5	3.5	5.3
164	7.3	8.2	12.4#

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:04:32 PM

