
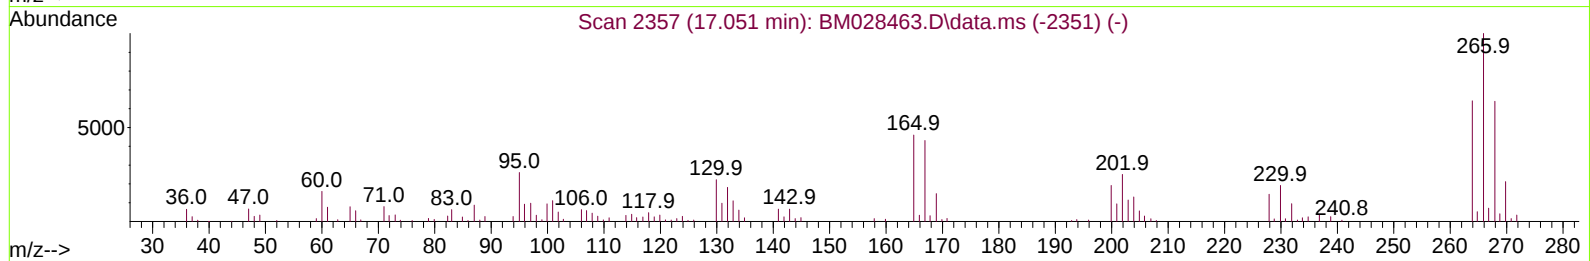
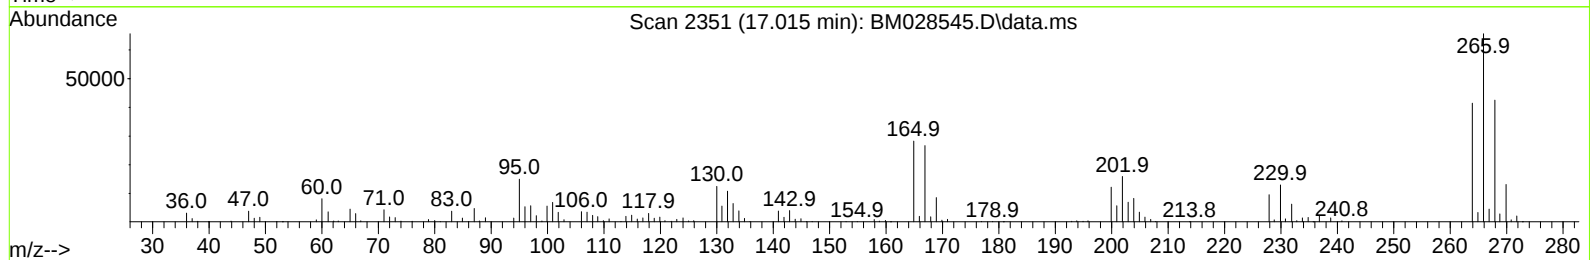


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028545.D
Acq On : 26 Jan 2021 17:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 07:16:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 03:11:35 2021
Response via : Initial Calibration

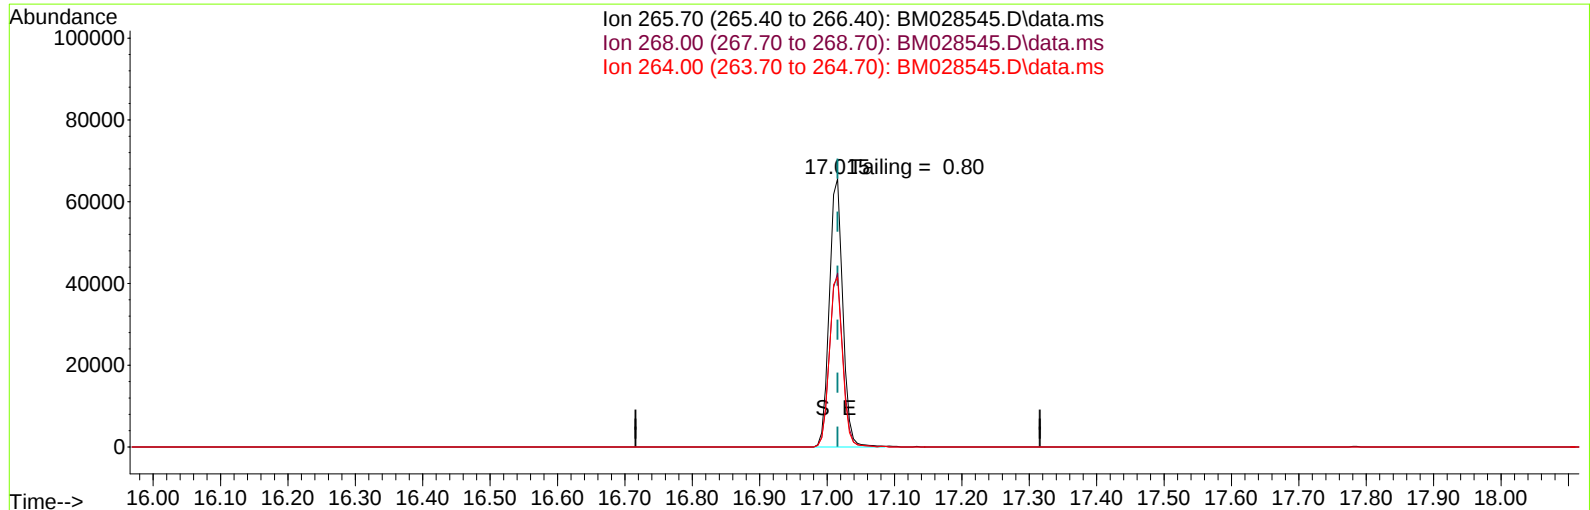

TIC: BM028545.D\data.ms

(70) Pentachlorophenol (C)




17.015min (-0.000) 0.00 ng

response 91360

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.79
264.00	63.30	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028545.D
Acq On : 26 Jan 2021 17:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 07:16:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 03:11:35 2021
Response via : Initial Calibration

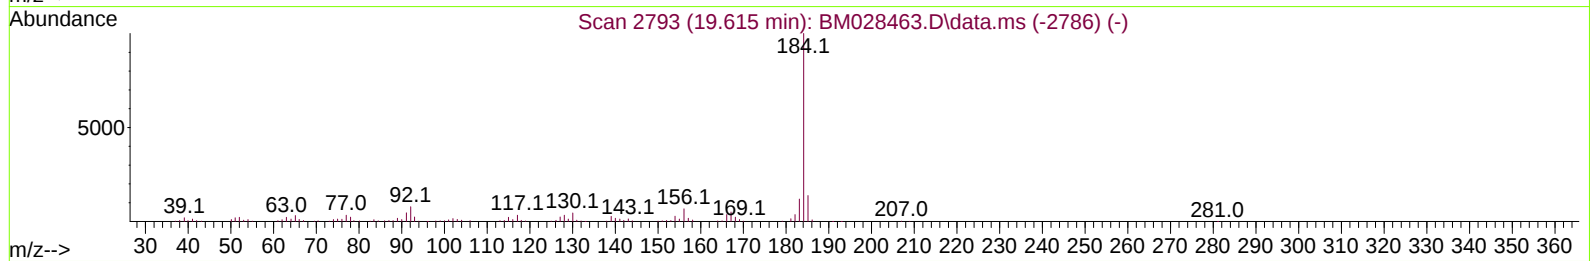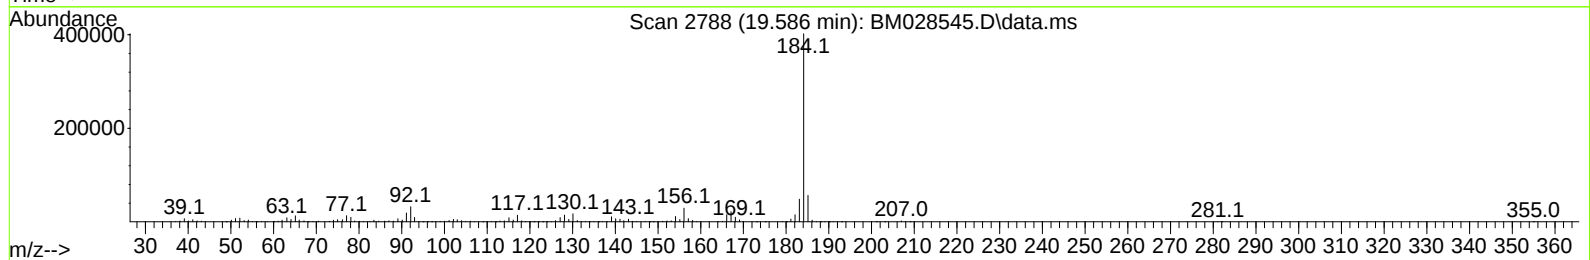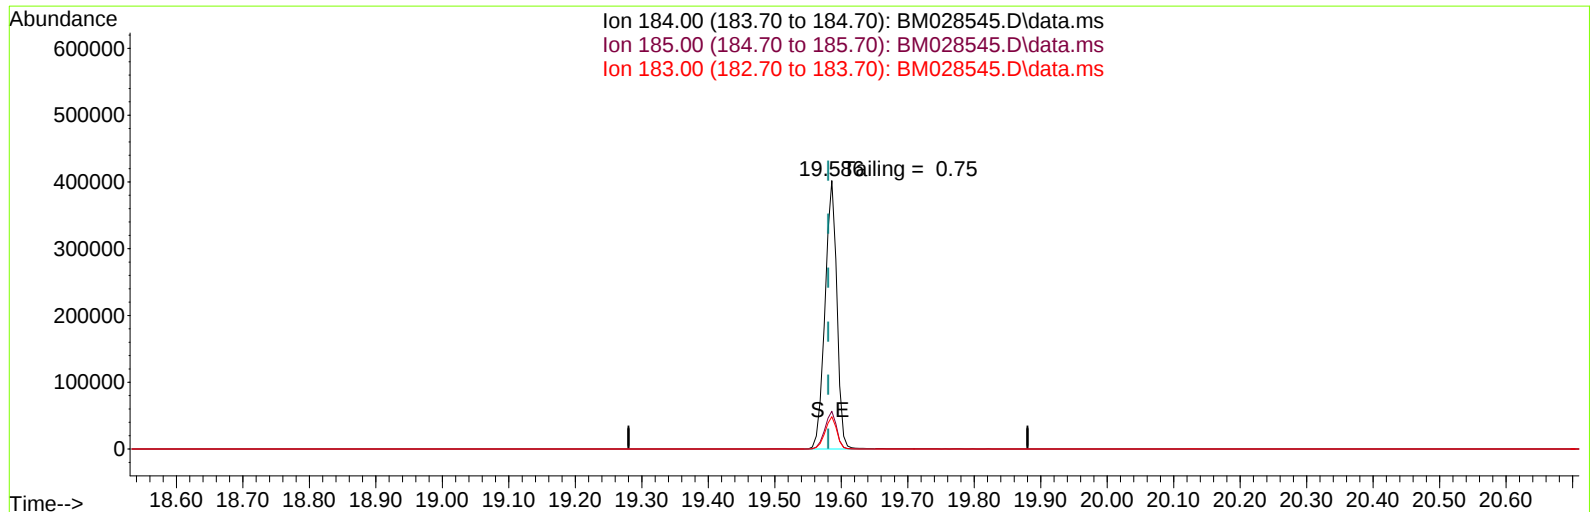

TIC: BM028545.D\data.ms

(77) Benzidine

19.586min (+ 0.006) 0.00 ng

response 500891

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.09
183.00	12.10	12.07
0.00	0.00	0.00