
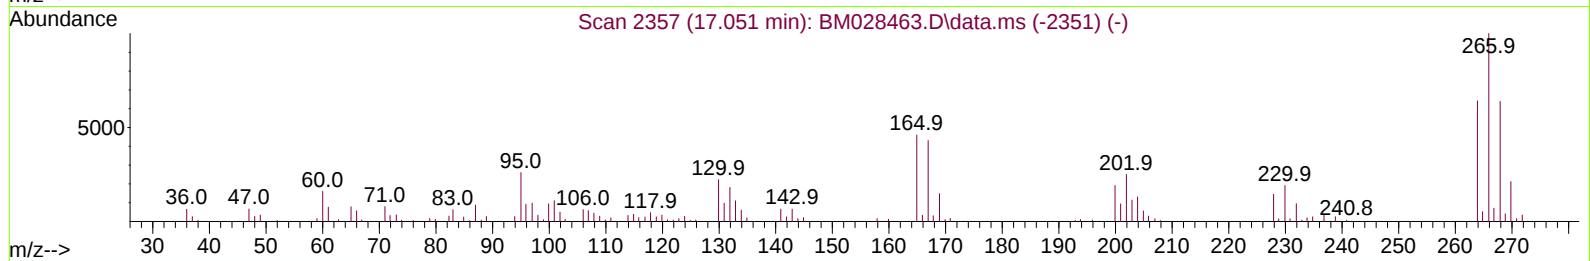
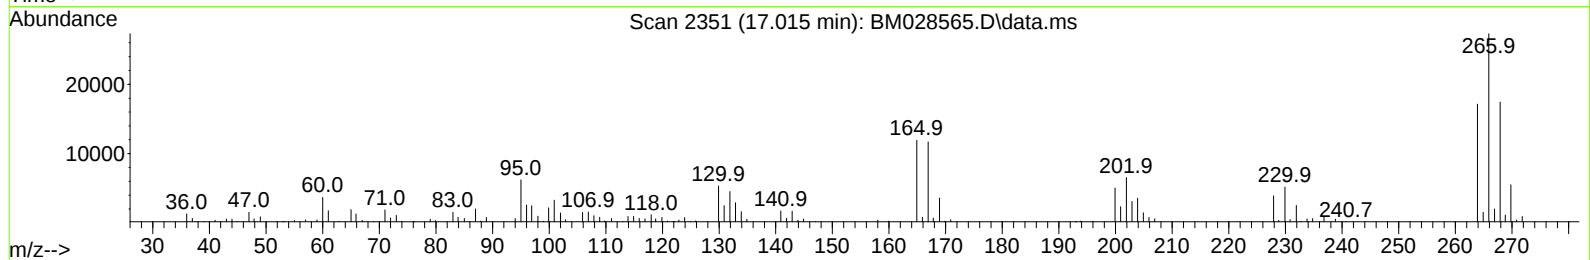


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028565.D
Acq On : 27 Jan 2021 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:38:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 13:20:04 2021
Response via : Initial Calibration

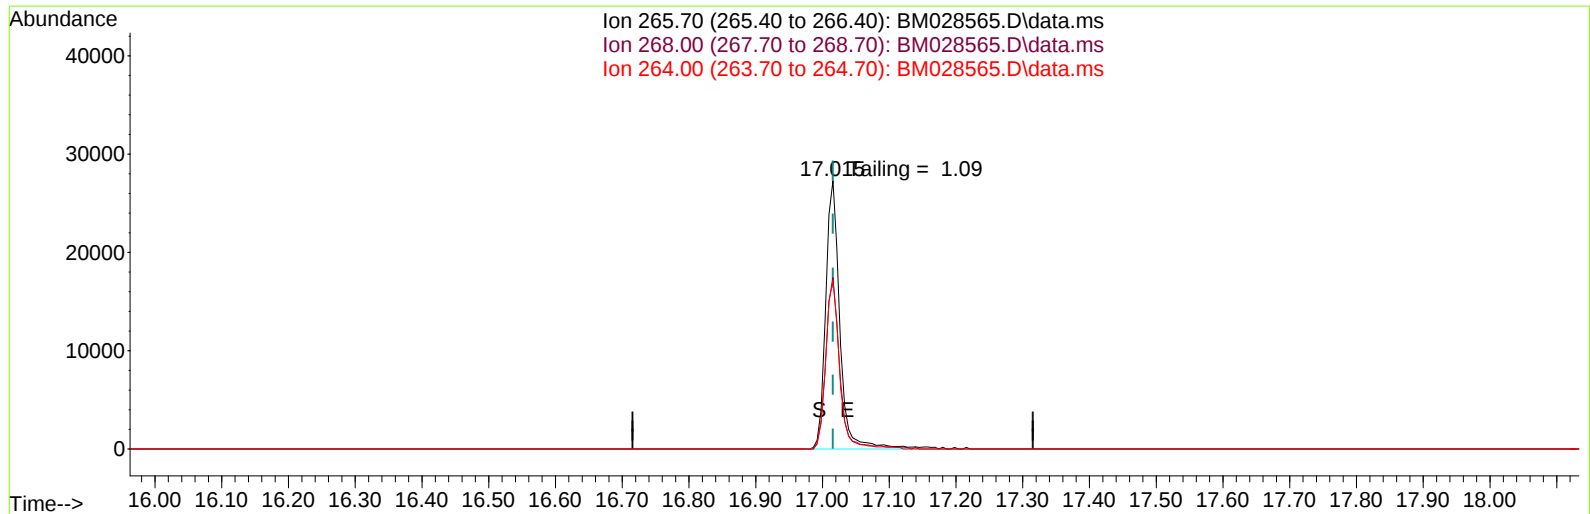

TIC: BM028565.D\data.ms

(70) Pentachlorophenol (C)




17.015min (+ 0.000) 0.00 ng

response 40252

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.84
264.00	63.30	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028565.D
Acq On : 27 Jan 2021 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:38:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 13:20:04 2021
Response via : Initial Calibration

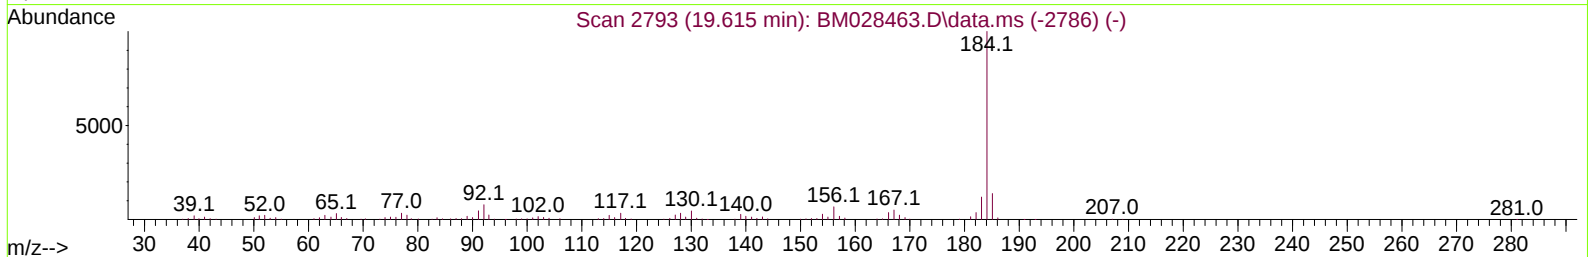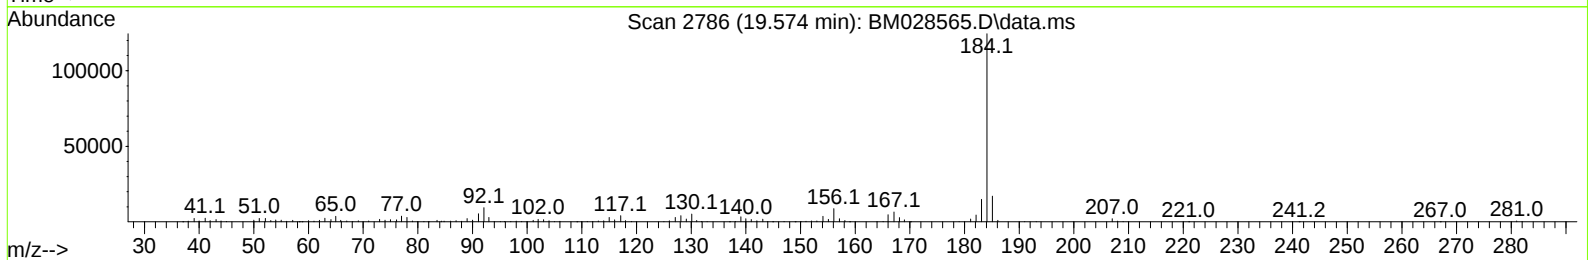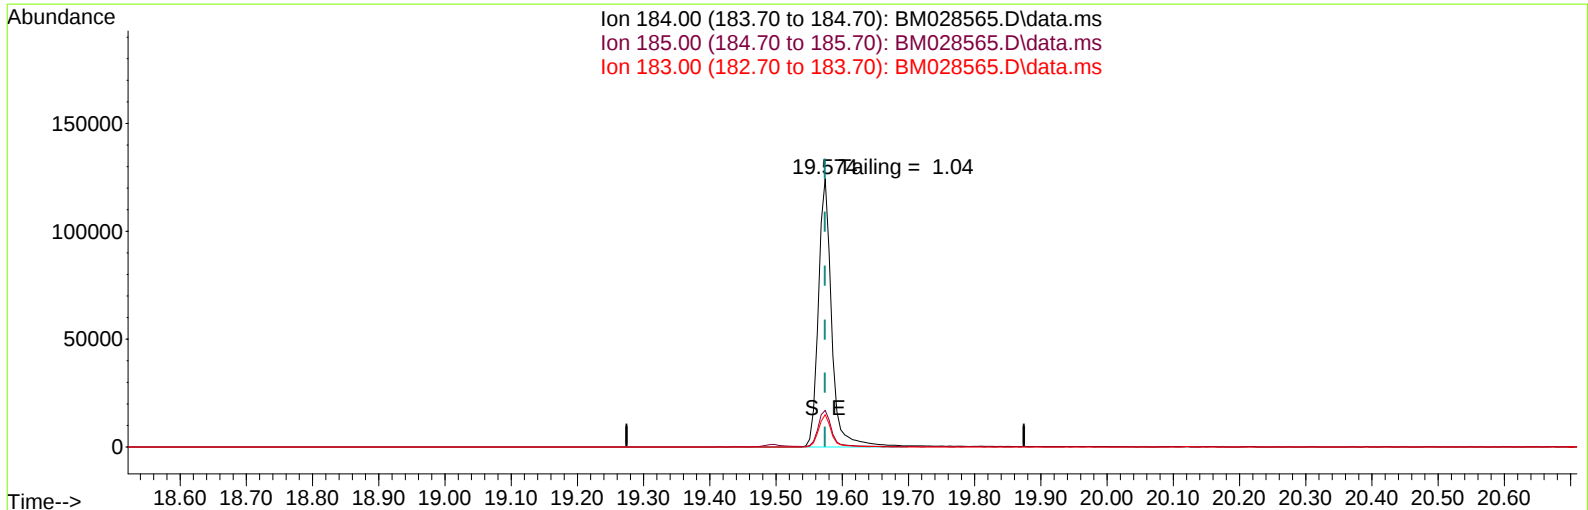

TIC: BM028565.D\data.ms

(77) Benzidine**19.574min (+ 0.000) 0.00 ng****response 174630**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.70
183.00	12.10	12.04
0.00	0.00	0.00