

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
 Data File : BM028547.D
 Acq On : 26 Jan 2021 18:56
 Operator : CG/JU
 Sample : PB134329BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134329BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	390	396	409	rVB	704193	997443	60.76%	11.788%
2	7.151	666	674	691	rBV	651589	1026932	62.56%	12.137%
3	7.993	810	817	823	rBB	121508	189270	11.53%	2.237%
4	9.169	1008	1017	1026	rBB	404265	668604	40.73%	7.902%
5	10.804	1288	1295	1303	rBB	160677	260204	15.85%	3.075%
6	13.257	1705	1712	1718	rBV	968860	1401902	85.40%	16.568%
7	14.633	1940	1946	1952	rVB	230195	319737	19.48%	3.779%
8	16.116	2192	2198	2204	rBV	720358	999734	60.90%	11.815%
9	17.363	2404	2410	2418	rVB	245580	340089	20.72%	4.019%
10	19.956	2845	2851	2856	rBV	1388113	1641617	100.00%	19.401%
11	21.492	3108	3112	3118	rBV	259048	319172	19.44%	3.772%
12	23.762	3492	3498	3507	rVB2	164352	296762	18.08%	3.507%




Sum of corrected areas: 8461466

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028547.D
Acq On : 26 Jan 2021 18:56
Operator : CG/JU
Sample : PB134329BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134329BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

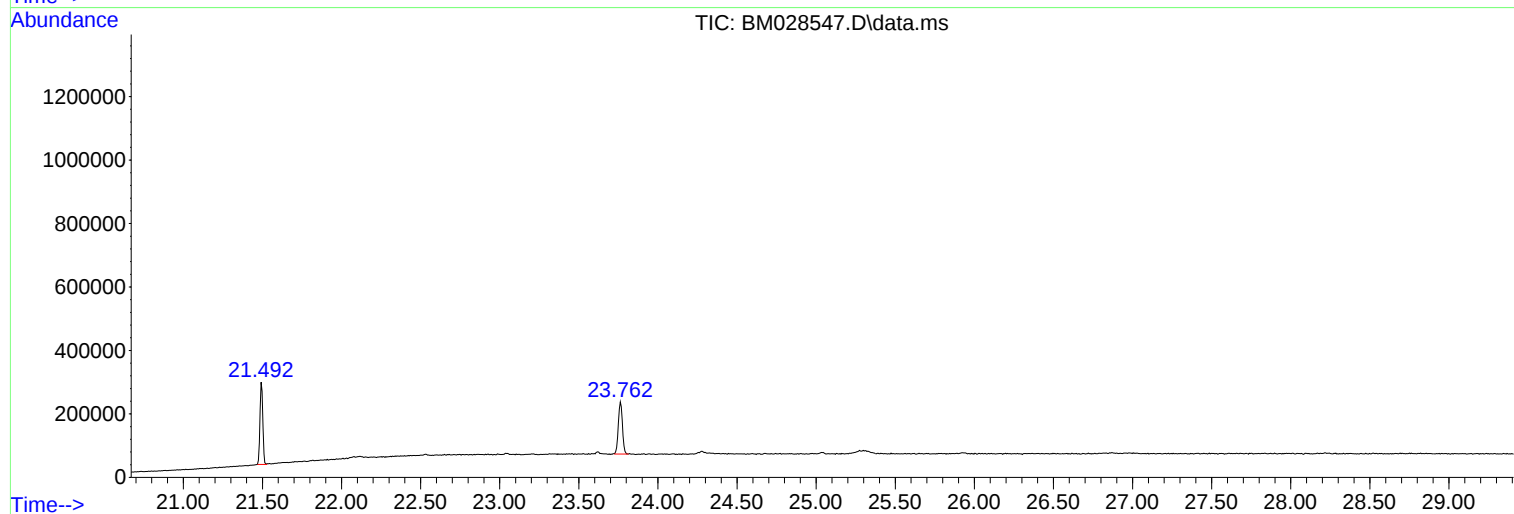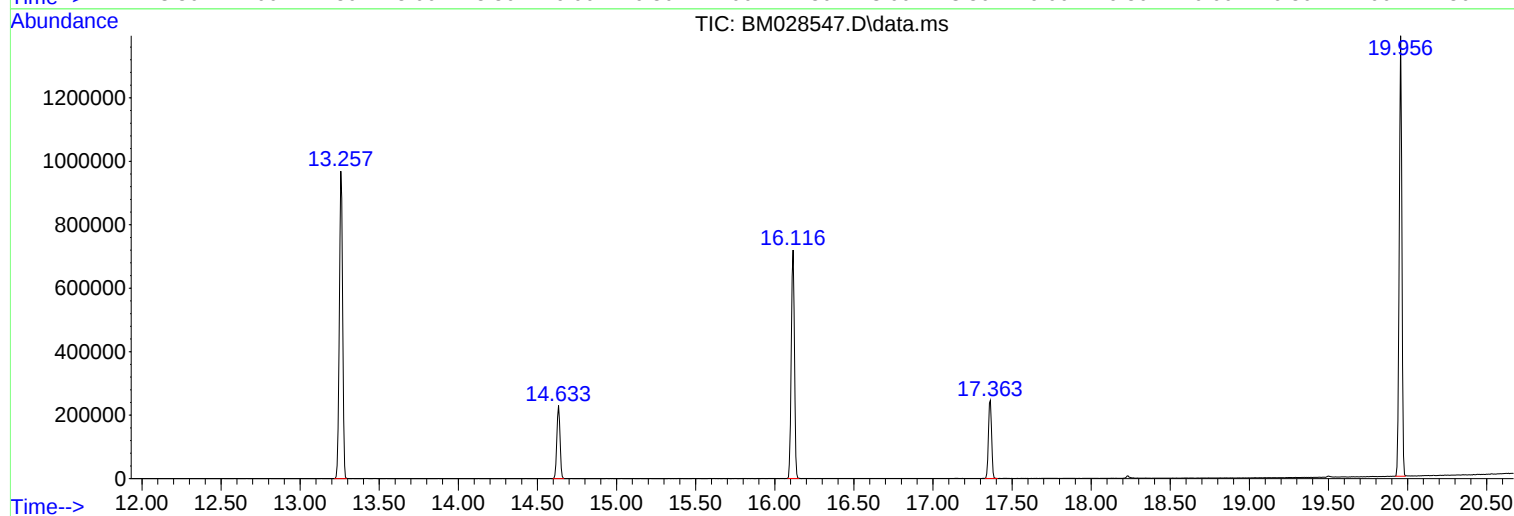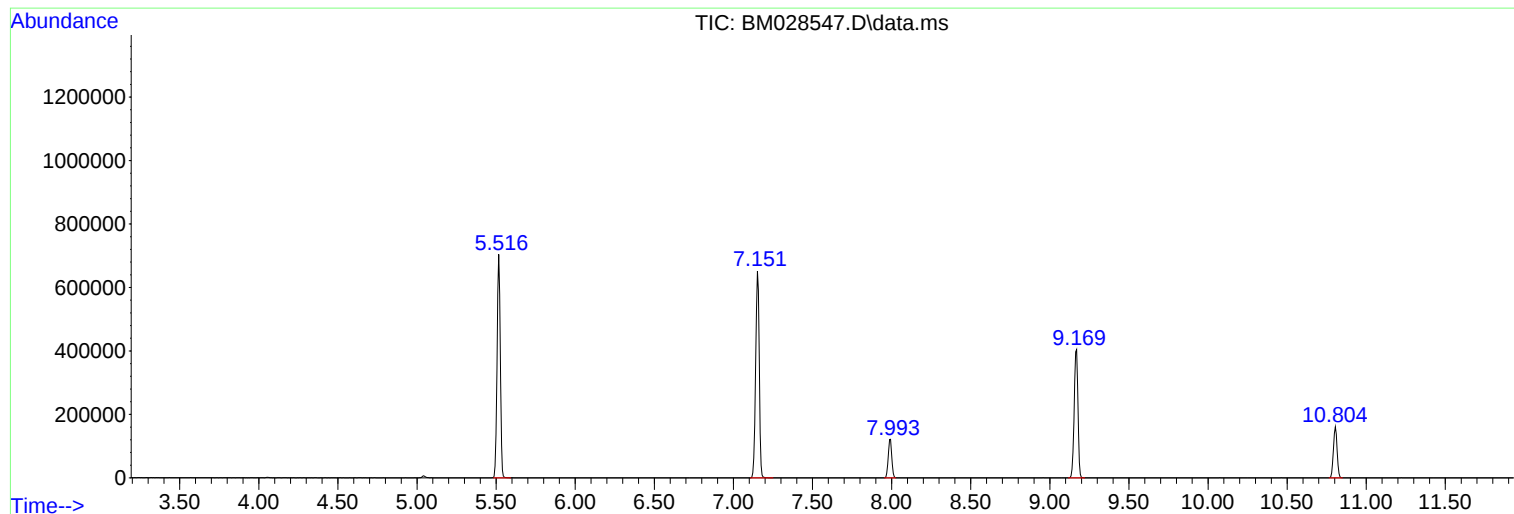

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028547.D
Acq On : 26 Jan 2021 18:56
Operator : CG/JU
Sample : PB134329BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134329BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028547.D
Acq On : 26 Jan 2021 18:56
Operator : CG/JU
Sample : PB134329BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134329BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------