

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
 Data File : BM028580.D
 Acq On : 27 Jan 2021 21:34
 Operator : CG/JU
 Sample : M1235-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FK-SF-SAMPLE-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	391	397	404	rBB	44178	62568	15.82%	2.344%
2	7.169	671	677	687	rBB	44507	71177	18.00%	2.667%
3	7.969	807	813	820	rVB	117995	181885	46.00%	6.814%
4	9.140	1006	1012	1019	rBV	26732	42184	10.67%	1.580%
5	10.781	1284	1291	1298	rVB	160169	252786	63.93%	9.470%
6	13.233	1702	1708	1714	rVB	68839	93490	23.64%	3.502%
7	13.428	1736	1741	1748	rVB2	3275	5302	1.34%	0.199%
8	14.080	1845	1852	1856	rVB2	3861	6489	1.64%	0.243%
9	14.498	1919	1923	1927	rVB3	4200	6206	1.57%	0.232%
10	14.616	1937	1943	1949	rVB2	218653	319583	80.82%	11.973%
11	15.445	2080	2084	2088	rBV2	4985	6305	1.59%	0.236%
12	15.845	2144	2152	2156	rBV3	3674	6785	1.72%	0.254%
13	16.098	2191	2195	2202	rBV	28387	35400	8.95%	1.326%
14	16.298	2223	2229	2231	rBV2	6511	9473	2.40%	0.355%
15	16.321	2231	2233	2239	rVB3	8456	10363	2.62%	0.388%
16	17.086	2359	2363	2366	rBV2	6219	7211	1.82%	0.270%
17	17.139	2367	2372	2375	rVV2	6693	9570	2.42%	0.359%
18	17.345	2401	2407	2412	rBV	263695	369129	93.35%	13.829%
19	17.386	2412	2414	2417	rVB	8728	9678	2.45%	0.363%
20	17.821	2484	2488	2493	rBV3	7086	8634	2.18%	0.323%
21	18.221	2551	2556	2560	rBV4	15871	26111	6.60%	0.978%
22	18.257	2560	2562	2568	rVB3	6526	8685	2.20%	0.325%
23	18.404	2583	2587	2590	rBV5	4173	6893	1.74%	0.258%
24	18.510	2601	2605	2611	rBV	6948	10904	2.76%	0.409%
25	18.998	2686	2688	2693	rBV6	2686	5014	1.27%	0.188%
26	19.133	2706	2711	2715	rBV4	10843	19378	4.90%	0.726%
27	19.386	2749	2754	2759	rBV	29431	43109	10.90%	1.615%
28	19.486	2769	2771	2775	rBV5	6494	8041	2.03%	0.301%
29	19.709	2806	2809	2811	rBV2	12077	14181	3.59%	0.531%
30	19.745	2811	2815	2822	rVB2	31609	52425	13.26%	1.964%
31	19.939	2844	2848	2852	rVB	125044	142526	36.04%	5.340%
32	21.180	3057	3059	3063	rVB	31384	33361	8.44%	1.250%
33	21.480	3106	3110	3115	rBV	311263	388976	98.37%	14.572%
34	23.750	3491	3496	3505	rVB2	215006	395435	100.00%	14.814%

Sum of corrected areas: 2669257

Instrument :

BNA_M

ClientSampleId :




FK-SF-SAMPLE-1

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028580.D
Acq On : 27 Jan 2021 21:34
Operator : CG/JU
Sample : M1235-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-SF-SAMPLE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

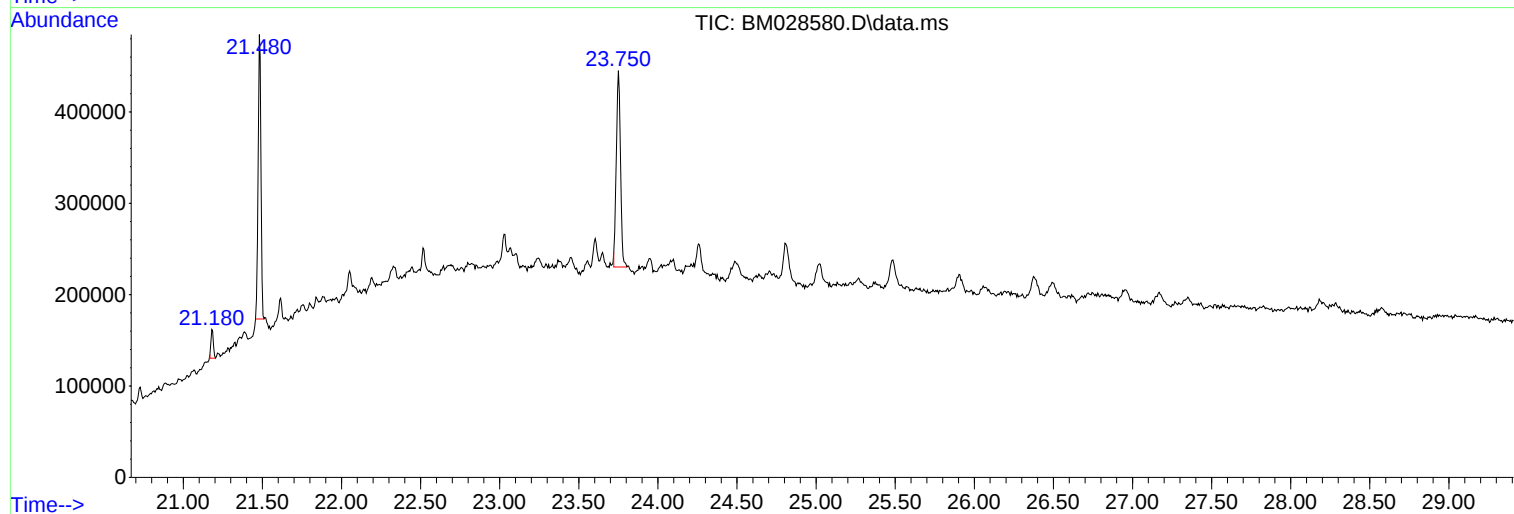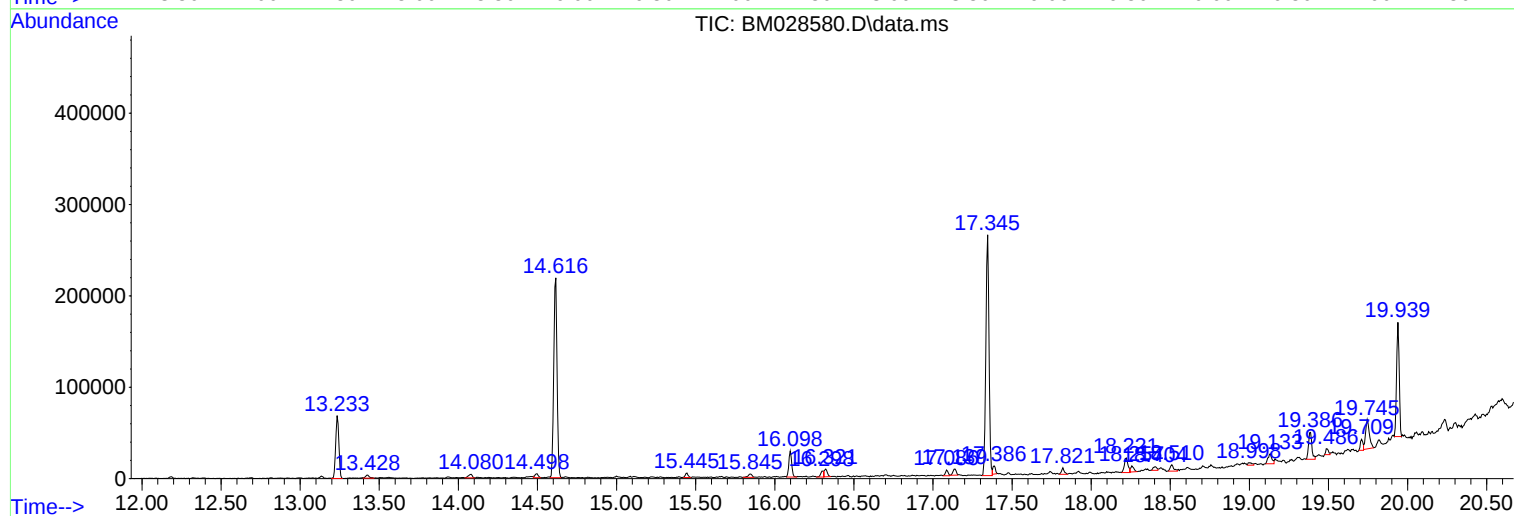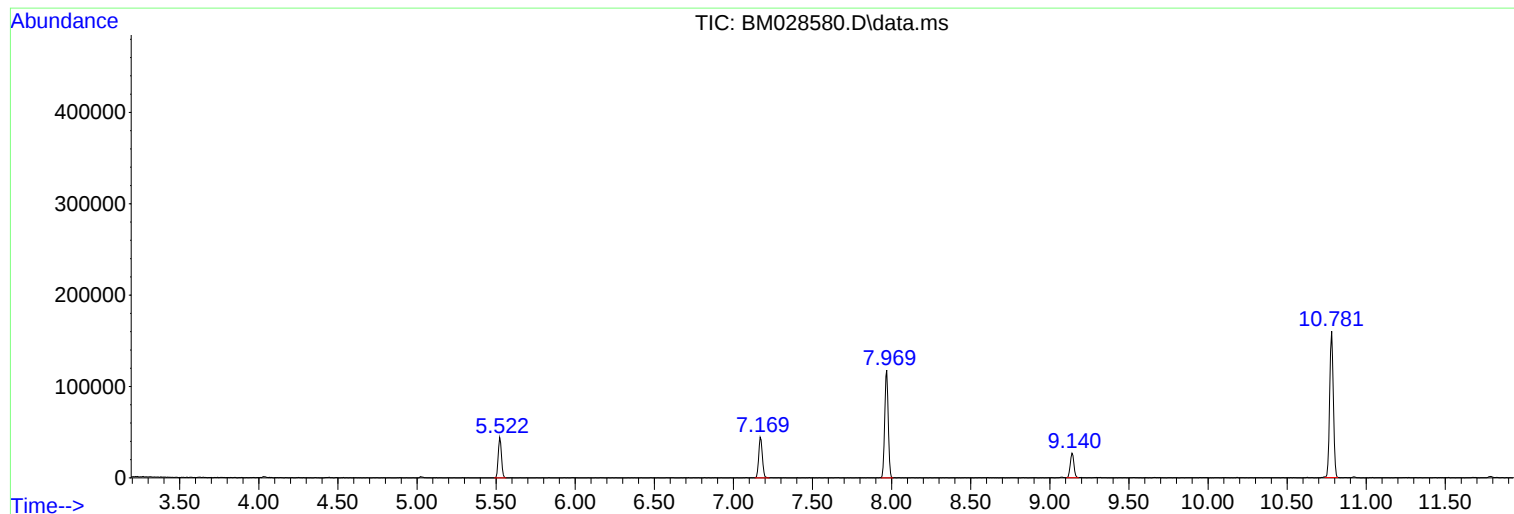

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028580.D
Acq On : 27 Jan 2021 21:34
Operator : CG/JU
Sample : M1235-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-SF-SAMPLE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028580.D
Acq On : 27 Jan 2021 21:34
Operator : CG/JU
Sample : M1235-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-SF-SAMPLE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------