

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
 Data File : BM028581.D
 Acq On : 27 Jan 2021 22:11
 Operator : CG/JU
 Sample : M1235-03 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FK-SF-SAMPLE-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	308	312	320	rBB	12628	17357	4.02%	0.651%
2	5.522	393	397	404	rBB	13011	18403	4.27%	0.690%
3	7.169	672	677	686	rVB	28151	43226	10.02%	1.620%
4	7.969	807	813	820	rBB	116625	178644	41.41%	6.697%
5	9.139	1005	1012	1019	rBV	18131	29004	6.72%	1.087%
6	10.780	1285	1291	1303	rVB	153545	246497	57.14%	9.240%
7	13.233	1703	1708	1715	rVB	44067	61521	14.26%	2.306%
8	14.468	1906	1918	1920	rBV4	1820	5127	1.19%	0.192%
9	14.615	1935	1943	1950	rVB	217307	310127	71.89%	11.625%
10	15.445	2079	2084	2088	rBV2	3818	4840	1.12%	0.181%
11	15.657	2115	2120	2127	rBV2	4959	7361	1.71%	0.276%
12	16.304	2226	2230	2231	rBV2	4987	6221	1.44%	0.233%
13	17.086	2359	2363	2367	rBV2	6651	8475	1.96%	0.318%
14	17.139	2367	2372	2374	rBV2	3563	4943	1.15%	0.185%
15	17.345	2401	2407	2411	rBV	253654	353759	82.01%	13.261%
16	17.386	2411	2414	2422	rVV	58369	78855	18.28%	2.956%
17	17.480	2425	2430	2434	rVB	10313	13991	3.24%	0.524%
18	17.751	2471	2476	2482	rBV	4806	7009	1.62%	0.263%
19	17.821	2484	2488	2491	rBV	7037	8068	1.87%	0.302%
20	17.921	2501	2505	2509	rVB2	4078	5127	1.19%	0.192%
21	18.221	2550	2556	2559	rBV2	14253	24972	5.79%	0.936%
22	18.262	2559	2563	2568	rVB	12214	17674	4.10%	0.663%
23	18.409	2581	2588	2592	rBV2	10222	21343	4.95%	0.800%
24	18.509	2601	2605	2610	rBV	8425	11444	2.65%	0.429%
25	18.756	2644	2647	2652	rVB6	7857	10439	2.42%	0.391%
26	19.133	2705	2711	2714	rBV5	14840	26115	6.05%	0.979%
27	19.386	2749	2754	2760	rBV	80888	109077	25.29%	4.089%
28	19.709	2806	2809	2811	rBV2	22173	25207	5.84%	0.945%
29	19.745	2811	2815	2822	rVB	69081	98638	22.87%	3.697%
30	19.939	2844	2848	2852	rVB2	83814	102499	23.76%	3.842%
31	21.480	3105	3110	3114	rBV	321843	431370	100.00%	16.170%
32	23.750	3491	3496	3503	rVB2	215309	380386	88.18%	14.259%




Sum of corrected areas: 2667719

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028581.D
Acq On : 27 Jan 2021 22:11
Operator : CG/JU
Sample : M1235-03 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-SF-SAMPLE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

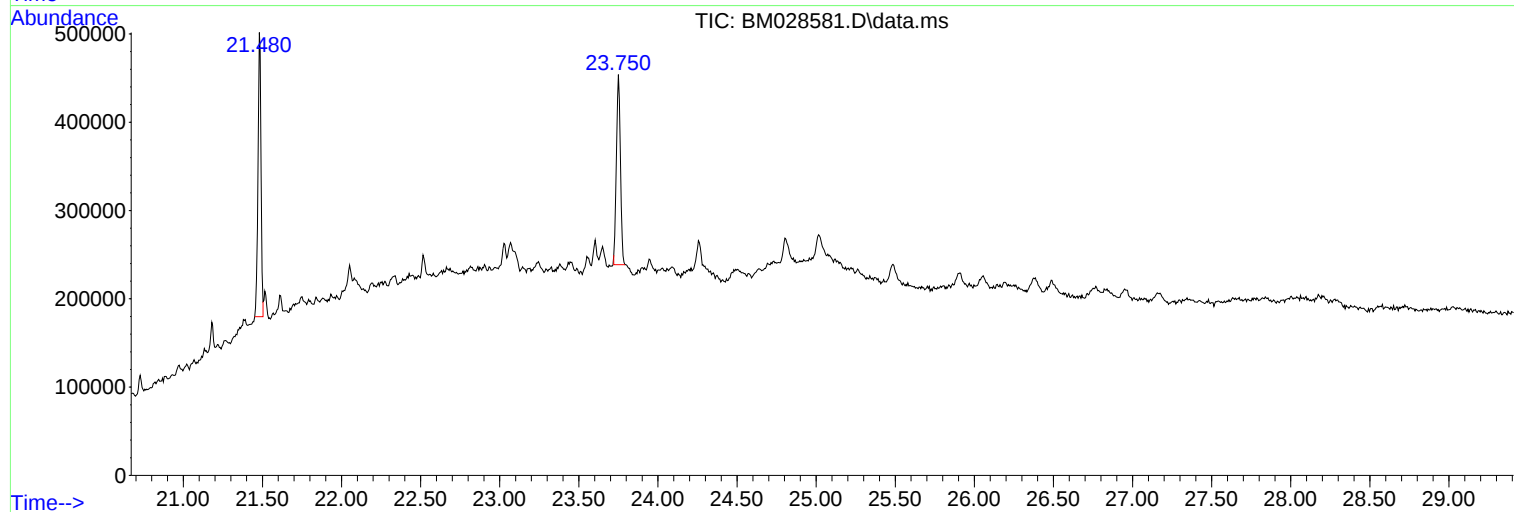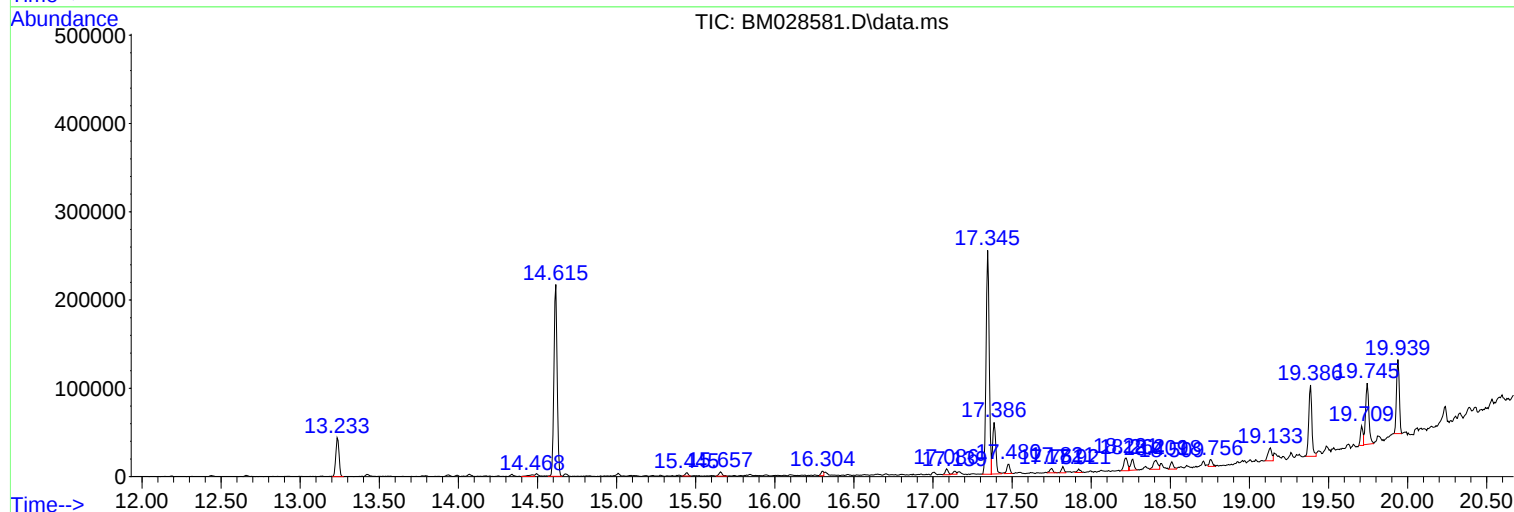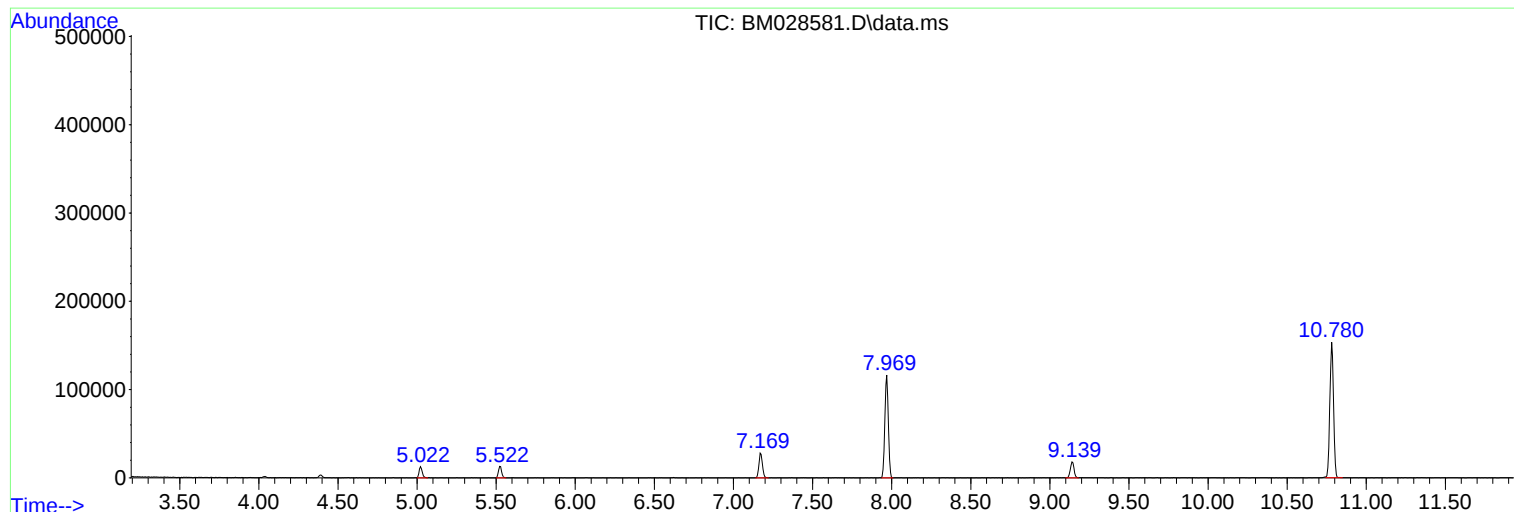

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028581.D
Acq On : 27 Jan 2021 22:11
Operator : CG/JU
Sample : M1235-03 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-SF-SAMPLE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
Data File : BM028581.D
Acq On : 27 Jan 2021 22:11
Operator : CG/JU
Sample : M1235-03 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-SF-SAMPLE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------