


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
 Data File : BM028545.D
 Acq On : 26 Jan 2021 17:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 27 03:11:35 2021

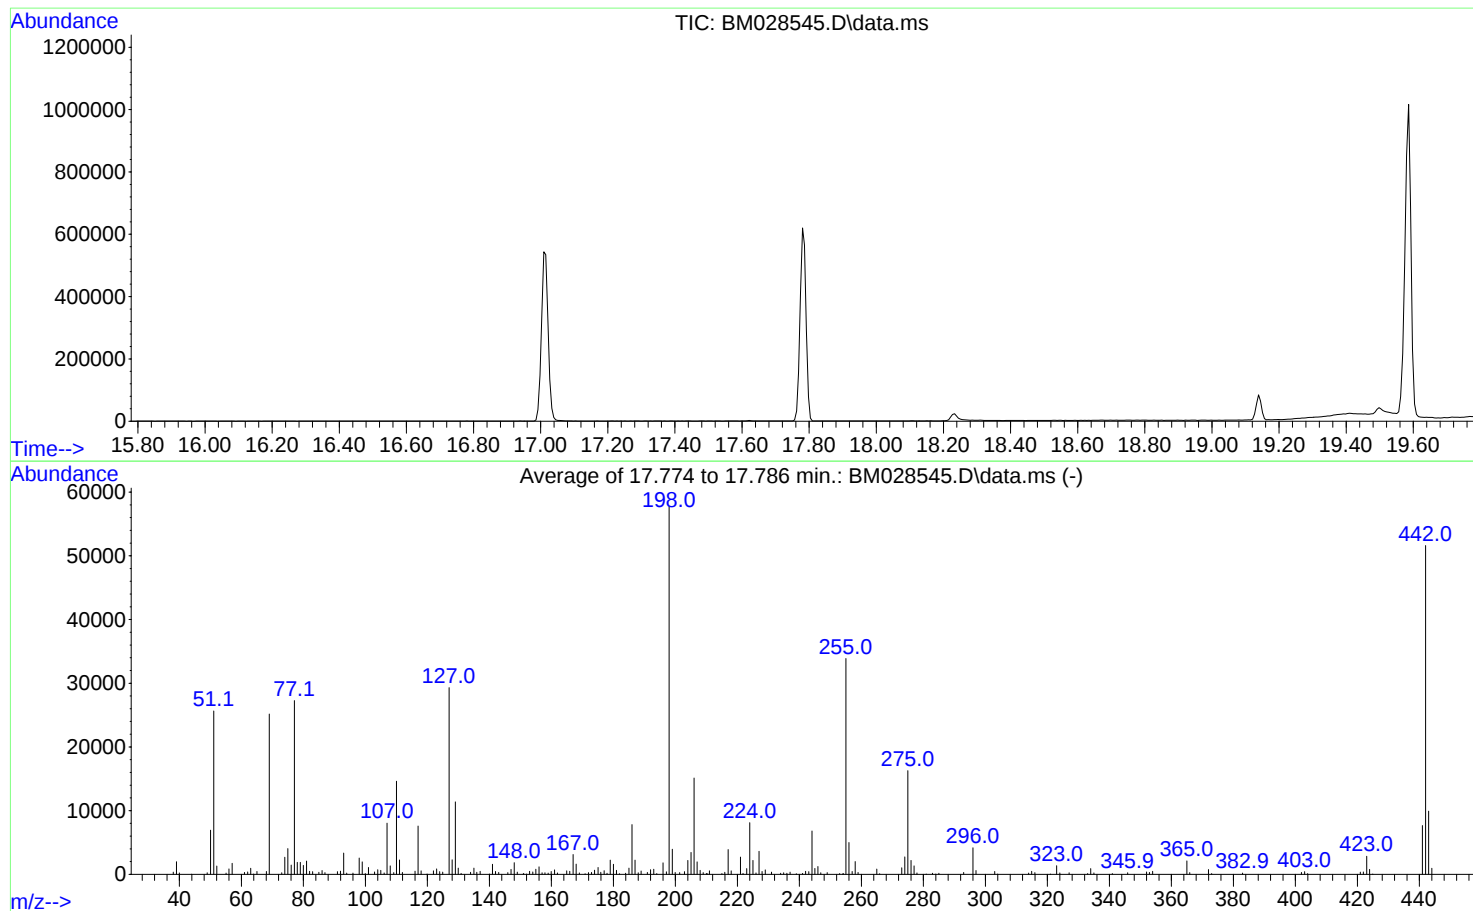

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	25653	PASS
68	69	0.00	2	1.8	450	PASS
69	198	0.00	100	43.6	25176	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	29301	PASS
197	198	0.00	2	0.7	415	PASS
198	198	100	100	100.0	57741	PASS
199	198	5	9	6.9	3957	PASS
275	198	10	60	28.2	16275	PASS
365	198	1	100	3.7	2110	PASS
441	198	0.01	100	13.3	7660	PASS
442	198	50	100	89.4	51611	PASS
443	442	15	24	19.2	9925	PASS