
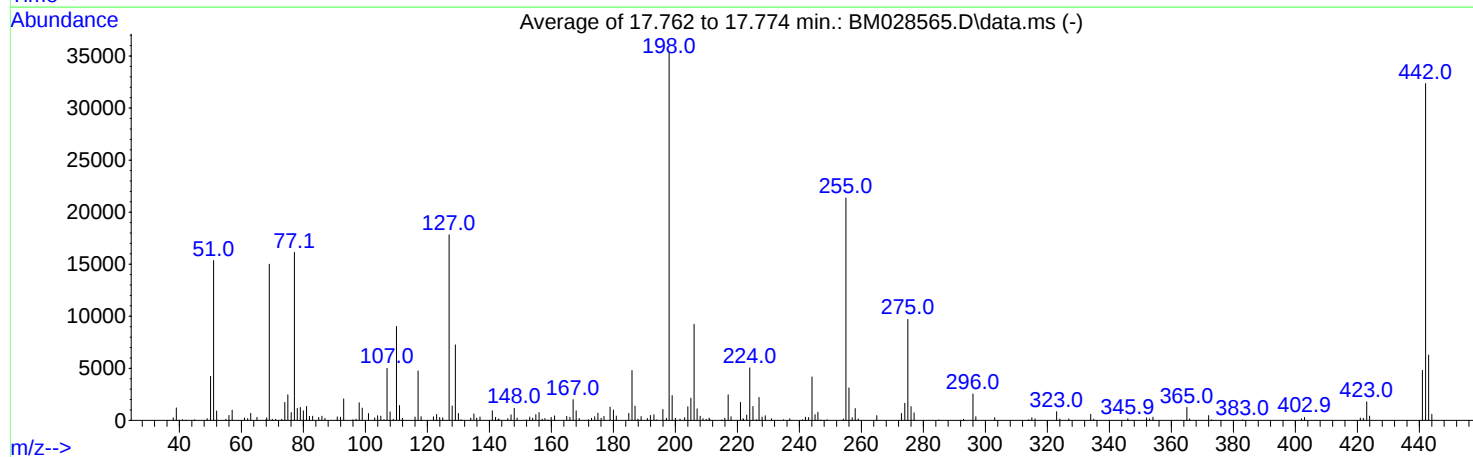


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012721\
 Data File : BM028565.D
 Acq On : 27 Jan 2021 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 27 13:20:04 2021

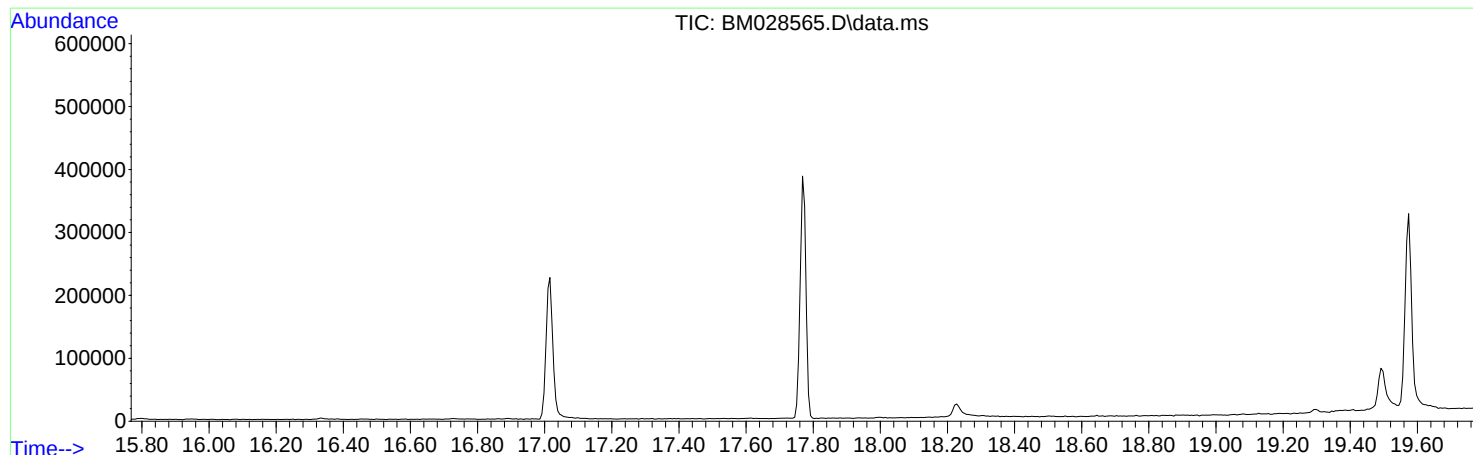

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	15364	PASS
68	69	0.00	2	1.6	243	PASS
69	198	0.00	100	42.4	14997	PASS
70	69	0.00	2	0.7	110	PASS
127	198	10	80	50.5	17832	PASS
197	198	0.00	2	0.6	195	PASS
198	198	100	100	100.0	35341	PASS
199	198	5	9	6.8	2390	PASS
275	198	10	60	27.5	9702	PASS
365	198	1	100	3.5	1245	PASS
441	198	0.01	100	13.6	4794	PASS
442	442	50	100	100.0	32363	PASS
443	442	15	24	19.4	6279	PASS