

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
 Data File : BM049445.D
 Acq On : 27 Jan 2025 10:30
 Operator : RC/JU
 Sample : PB166251BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	31	rVB	59542	83325	2.63%	0.240%
2	3.504	84	88	100	rBV	710531	1045356	33.00%	3.017%
3	6.710	625	633	644	rBV	705613	1119199	35.33%	3.230%
4	6.863	653	659	674	rVB	561967	872574	27.54%	2.518%
5	7.057	685	692	704	rBV	714511	1106916	34.94%	3.194%
6	7.157	706	709	712	rVB5	2893	3793	0.12%	0.011%
7	7.516	763	770	780	rBV	572758	910315	28.74%	2.627%
8	8.228	884	891	908	rBV	788377	1248358	39.41%	3.602%
9	8.657	957	964	977	rBV	585708	948517	29.94%	2.737%
10	9.039	1024	1029	1030	rBV4	3416	4998	0.16%	0.014%
11	9.375	1079	1086	1097	rBV	433213	723455	22.84%	2.088%
12	9.716	1142	1144	1148	rBV6	2718	3437	0.11%	0.010%
13	9.910	1170	1177	1194	rBV	683861	1206196	38.08%	3.481%
14	10.275	1232	1239	1247	rBV	709545	1148024	36.24%	3.313%
15	10.422	1257	1264	1286	rBV	568053	1123587	35.47%	3.242%
16	11.886	1509	1513	1519	rBV5	6170	13448	0.42%	0.039%
17	13.574	1794	1800	1812	rBV	1170882	1651961	52.15%	4.767%
18	13.845	1839	1846	1860	rBV	1374954	2038992	64.37%	5.884%
19	14.157	1892	1899	1907	rBV	982563	1450216	45.78%	4.185%
20	14.386	1931	1938	1949	rBV	199973	487388	15.39%	1.406%
21	15.157	2061	2069	2083	rBV	1764225	2505148	79.08%	7.229%
22	15.280	2085	2090	2107	rVV	418505	617809	19.50%	1.783%
23	15.398	2107	2110	2117	rVB5	7820	11781	0.37%	0.034%
24	16.592	2311	2313	2320	rVB7	2192	3744	0.12%	0.011%
25	16.698	2327	2331	2335	rVB3	4155	6461	0.20%	0.019%
26	16.904	2360	2366	2376	rBV2	1277969	1698587	53.62%	4.902%
27	17.004	2377	2383	2403	rVB	1991471	2695554	85.09%	7.779%
28	17.845	2520	2526	2527	rBV6	2481	4215	0.13%	0.012%
29	18.874	2697	2701	2706	rVB5	18872	27606	0.87%	0.080%
30	18.945	2708	2713	2718	rVV2	15837	24659	0.78%	0.071%
31	19.309	2769	2775	2788	rBV	2432133	3167813	100.00%	9.142%
32	21.133	3080	3085	3099	rBV	1270737	1827347	57.68%	5.273%
33	23.721	3518	3525	3539	rVB	1332254	2961983	93.50%	8.548%
34	23.915	3550	3558	3570	rVB	839802	1909819	60.29%	5.511%

Sum of corrected areas: 34652581

Instrument :

BNA_M

ClientSampleId :




SBLK251

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049445.D
Acq On : 27 Jan 2025 10:30
Operator : RC/JU
Sample : PB166251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

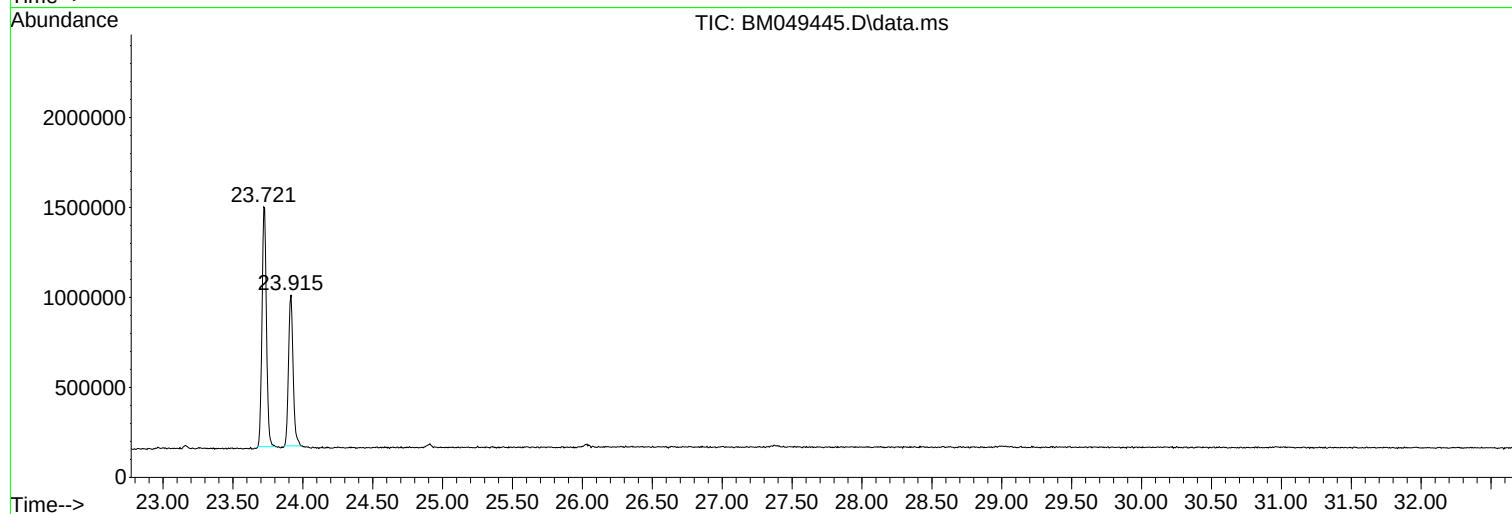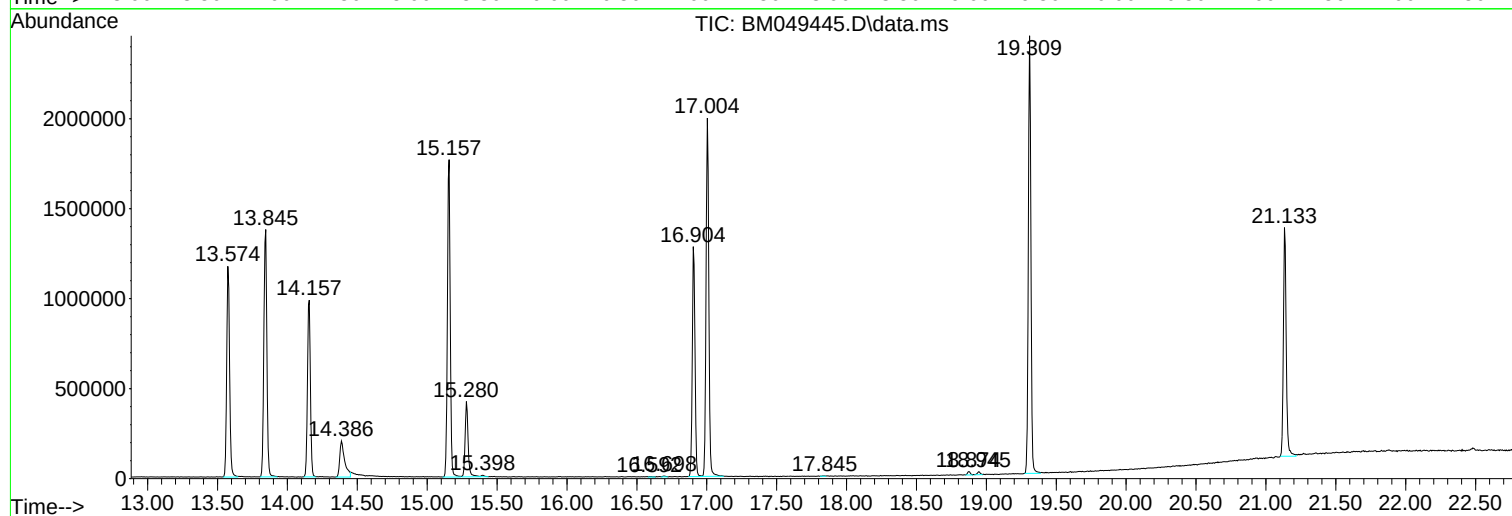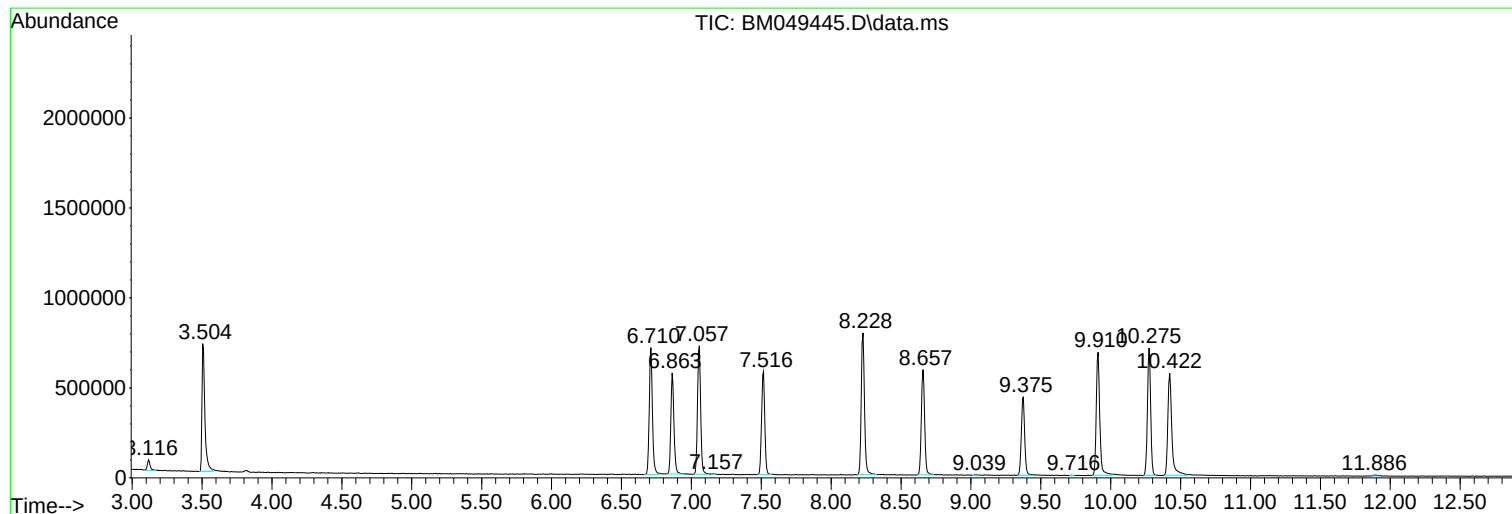

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049445.D
Acq On : 27 Jan 2025 10:30
Operator : RC/JU
Sample : PB166251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049445.D
Acq On : 27 Jan 2025 10:30
Operator : RC/JU
Sample : PB166251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc