

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
 Data File : BM049451.D
 Acq On : 27 Jan 2025 16:44
 Operator : RC/JU
 Sample : PB166231BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	19	22	33	rVB	61353	84585	2.50%	0.235%
2	3.510	85	89	103	rBV	777001	1141015	33.73%	3.164%
3	3.810	137	140	147	rVB6	11287	19274	0.57%	0.053%
4	4.434	244	246	250	rBV5	4082	4538	0.13%	0.013%
5	5.451	418	419	424	rBV4	3158	3593	0.11%	0.010%
6	6.710	625	633	648	rBV	757048	1203441	35.57%	3.337%
7	6.863	653	659	673	rVB	606371	951733	28.13%	2.639%
8	7.057	685	692	706	rBV	770512	1207196	35.69%	3.348%
9	7.187	712	714	718	rVB5	3217	3601	0.11%	0.010%
10	7.410	748	752	754	rVB5	3023	3987	0.12%	0.011%
11	7.516	763	770	778	rBV	546380	872691	25.80%	2.420%
12	8.228	884	891	905	rBV	839983	1342876	39.70%	3.724%
13	8.657	957	964	975	rBV	639136	1036288	30.63%	2.874%
14	9.063	1030	1033	1037	rBV6	3928	5664	0.17%	0.016%
15	9.369	1078	1085	1096	rBV	479029	801524	23.69%	2.223%
16	9.910	1169	1177	1194	rBV	762739	1323794	39.13%	3.671%
17	10.275	1231	1239	1250	rBV	676126	1100016	32.52%	3.050%
18	10.422	1256	1264	1282	rBV	609040	1191683	35.23%	3.305%
19	11.886	1508	1513	1515	rBV4	5817	9218	0.27%	0.026%
20	13.574	1794	1800	1813	rBV	1254251	1762174	52.09%	4.887%
21	13.845	1839	1846	1860	rBV	1502643	2201628	65.08%	6.105%
22	14.151	1892	1898	1913	rVB	933627	1380074	40.80%	3.827%
23	14.386	1932	1938	1964	rBV	217149	611269	18.07%	1.695%
24	15.157	2062	2069	2080	rBV	1893324	2672260	78.99%	7.410%
25	15.280	2085	2090	2106	rVV	431467	633085	18.71%	1.756%
26	15.392	2106	2109	2114	rVB4	6425	11722	0.35%	0.033%
27	16.698	2326	2331	2333	rVB3	2809	3584	0.11%	0.010%
28	16.904	2360	2366	2377	rBV2	1143987	1596020	47.18%	4.426%
29	17.004	2377	2383	2399	rVV	2066642	2863154	84.64%	7.940%
30	17.109	2399	2401	2411	rVV8	5305	9432	0.28%	0.026%
31	17.503	2467	2468	2473	rBV4	2922	3627	0.11%	0.010%
32	17.598	2478	2484	2487	rVV6	3747	5746	0.17%	0.016%
33	17.845	2525	2526	2532	rVB5	2645	3393	0.10%	0.009%
34	18.874	2697	2701	2707	rVB5	20765	29617	0.88%	0.082%
35	18.945	2707	2713	2720	rBV2	20436	32661	0.97%	0.091%
36	19.133	2741	2745	2751	rBV8	5940	12936	0.38%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049451.D
Acq On : 27 Jan 2025 16:44
Operator : RC/JU
Sample : PB166231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK231

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Title : SVOA CALIBRATION

37	19.309	2769	2775	2787	rBV	2558478	3382869	100.00%	9.381%
38	21.139	3080	3086	3096	rBV	1149824	1661056	49.10%	4.606%
39	23.727	3518	3526	3539	rBV	1483640	3093644	91.45%	8.579%
40	23.915	3551	3558	3573	rVB	763401	1785141	52.77%	4.950%




Sum of corrected areas: 36061809

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049451.D
Acq On : 27 Jan 2025 16:44
Operator : RC/JU
Sample : PB166231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK231

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

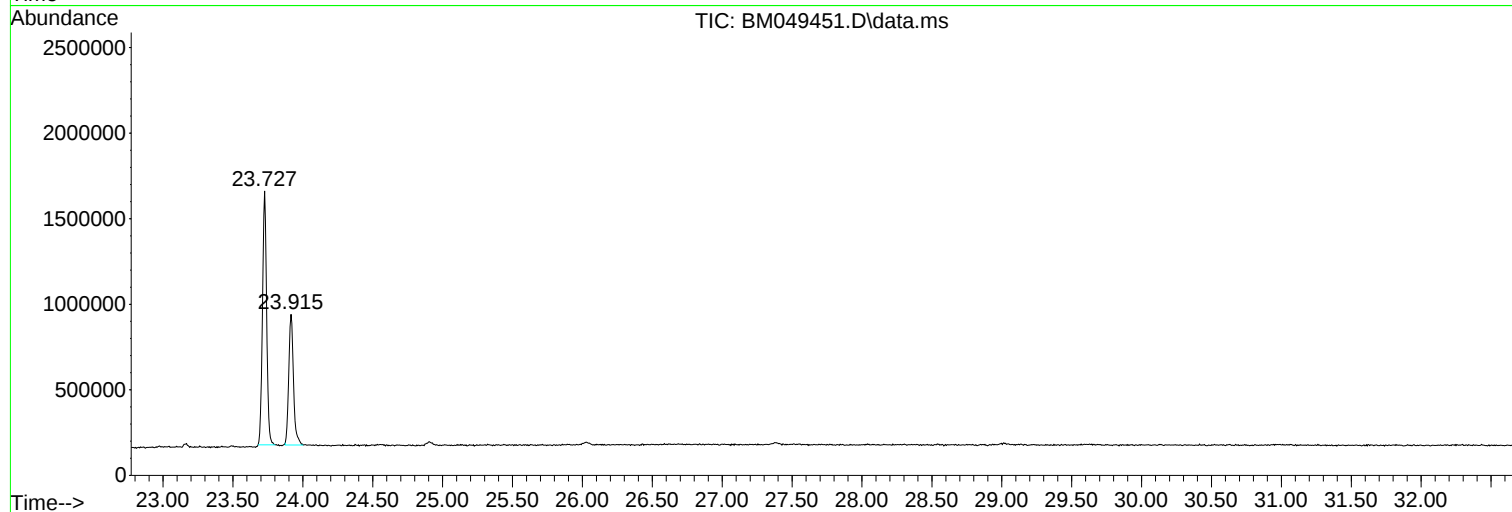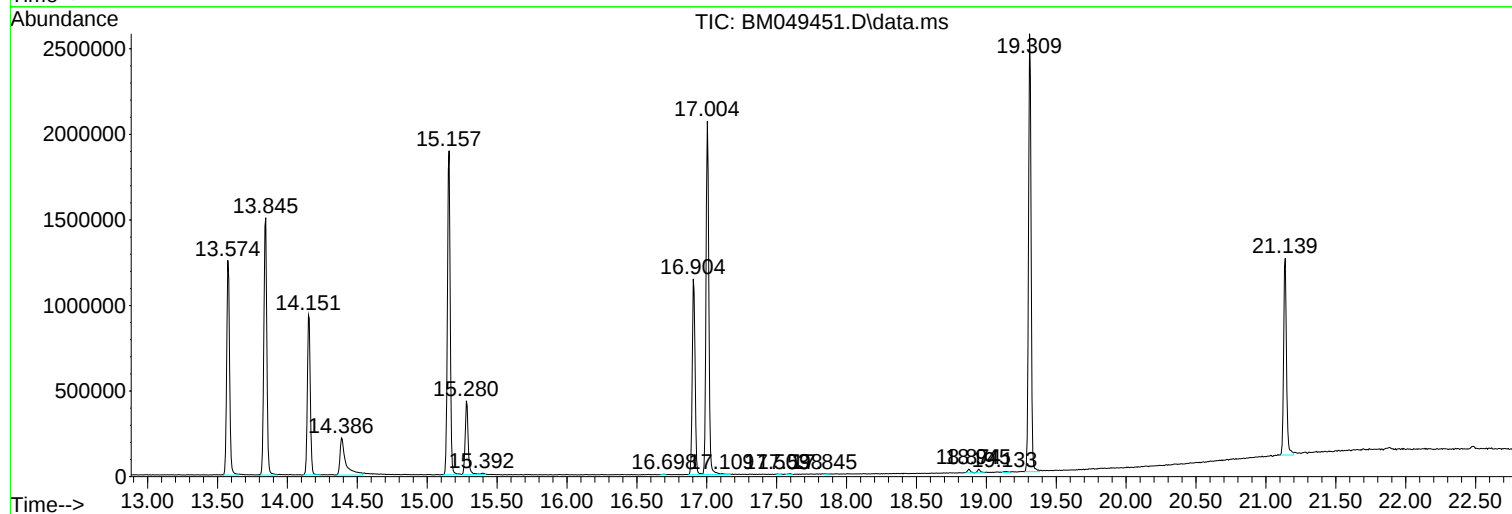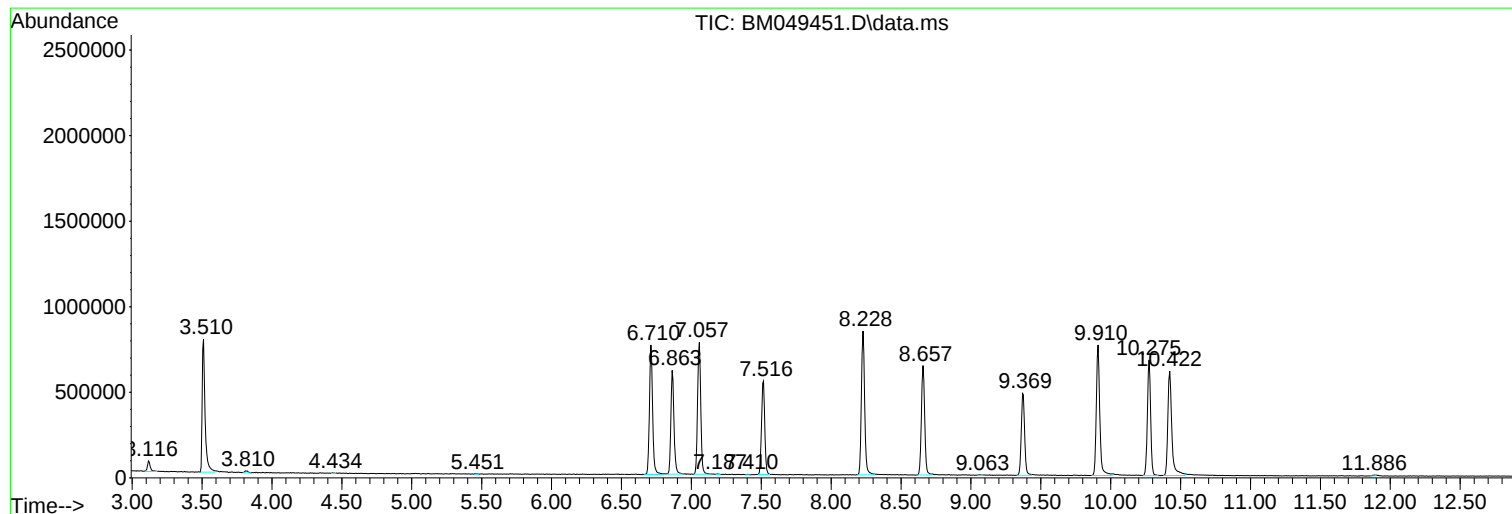

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049451.D
Acq On : 27 Jan 2025 16:44
Operator : RC/JU
Sample : PB166231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK231

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049451.D
Acq On : 27 Jan 2025 16:44
Operator : RC/JU
Sample : PB166231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK231

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc