

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
 Data File : BM049452.D
 Acq On : 27 Jan 2025 17:23
 Operator : RC/JU
 Sample : PB166251BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	30	rVB	64083	80632	2.30%	0.216%
2	3.504	84	88	108	rBV	778148	1120244	31.96%	2.995%
3	3.810	138	140	148	rVB5	11503	17111	0.49%	0.046%
4	6.710	626	633	649	rBV	748827	1182396	33.73%	3.161%
5	6.863	653	659	670	rVV	588920	913354	26.06%	2.442%
6	7.057	685	692	706	rBV	767928	1166588	33.28%	3.119%
7	7.510	762	769	779	rBV	594658	948358	27.05%	2.536%
8	8.045	858	860	864	rVB4	2736	3507	0.10%	0.009%
9	8.228	884	891	907	rBV	840909	1320509	37.67%	3.530%
10	8.657	957	964	976	rBV	616494	1007395	28.74%	2.693%
11	9.375	1078	1086	1097	rBV	465364	771924	22.02%	2.064%
12	9.910	1166	1177	1192	rBV	733436	1293380	36.90%	3.458%
13	10.275	1232	1239	1253	rBV	748387	1198879	34.20%	3.205%
14	10.422	1255	1264	1284	rBV	616445	1187261	33.87%	3.174%
15	11.892	1509	1514	1521	rVB4	6318	15718	0.45%	0.042%
16	12.033	1533	1538	1544	rVB7	2550	4887	0.14%	0.013%
17	13.574	1792	1800	1816	rBV	1228587	1736667	49.54%	4.643%
18	13.845	1839	1846	1865	rBV	1491336	2160274	61.63%	5.776%
19	14.151	1892	1898	1909	rBV	1067532	1556009	44.39%	4.160%
20	14.386	1932	1938	1965	rBV2	221748	615349	17.55%	1.645%
21	14.833	2012	2014	2019	rVB5	4409	5277	0.15%	0.014%
22	15.157	2062	2069	2085	rBV	1949082	2697455	76.95%	7.212%
23	15.280	2085	2090	2103	rBV	370572	549186	15.67%	1.468%
24	15.398	2108	2110	2119	rVB4	9395	11174	0.32%	0.030%
25	16.698	2326	2331	2333	rBV3	4406	6198	0.18%	0.017%
26	16.904	2360	2366	2377	rBV2	1295112	1823978	52.03%	4.877%
27	17.004	2377	2383	2398	rVV	2076360	2891301	82.48%	7.730%
28	18.880	2698	2702	2707	rVB3	18965	26460	0.75%	0.071%
29	18.951	2709	2714	2718	rBV2	17627	27180	0.78%	0.073%
30	19.309	2765	2775	2788	rBV	2613200	3505297	100.00%	9.372%
31	21.139	3080	3086	3096	rBV	1354981	1960163	55.92%	5.241%
32	23.727	3517	3526	3542	rBV	1514911	3372941	96.22%	9.018%
33	23.915	3550	3558	3576	rVB	892305	2226034	63.50%	5.951%




Sum of corrected areas: 37403086

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049452.D
Acq On : 27 Jan 2025 17:23
Operator : RC/JU
Sample : PB166251BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

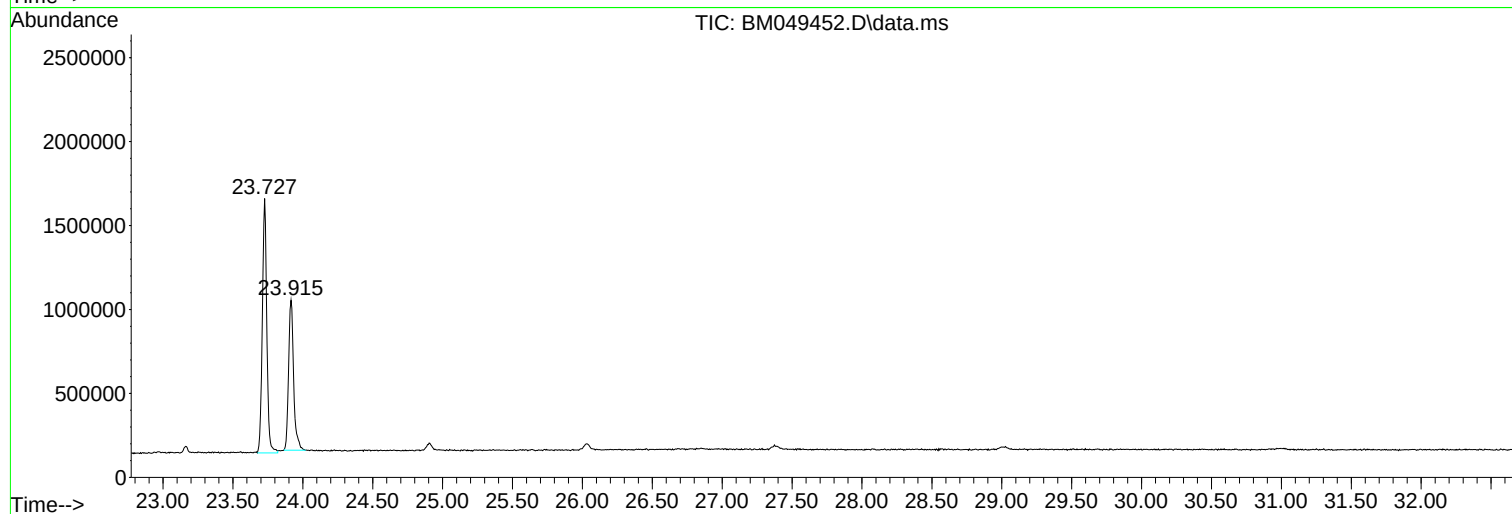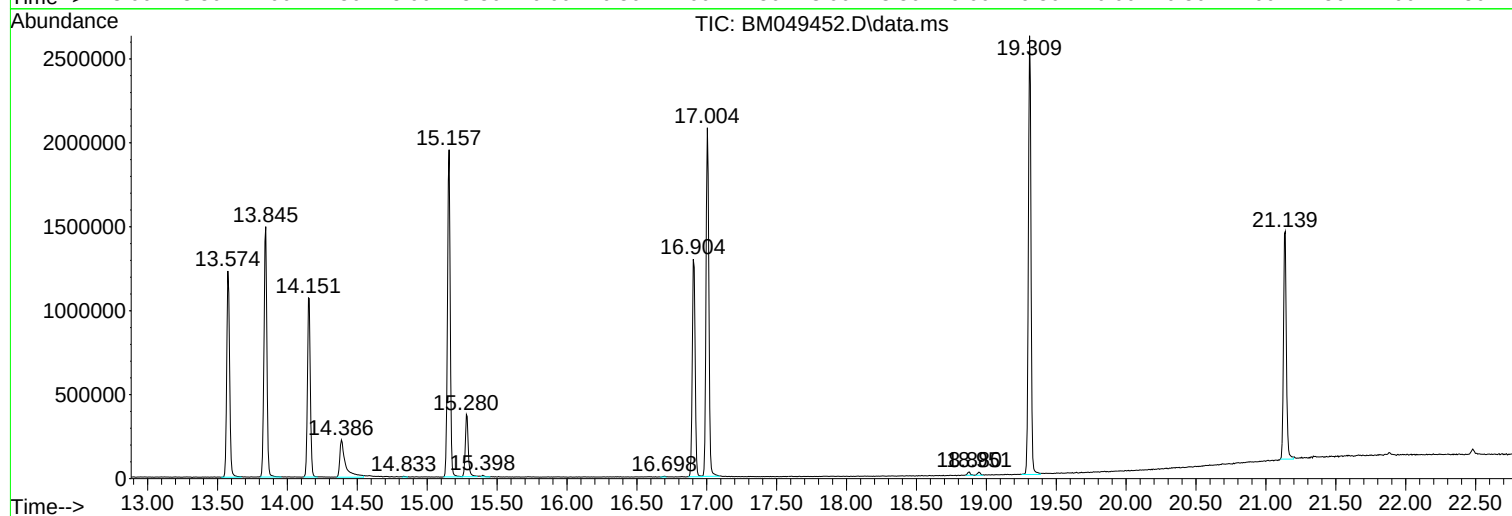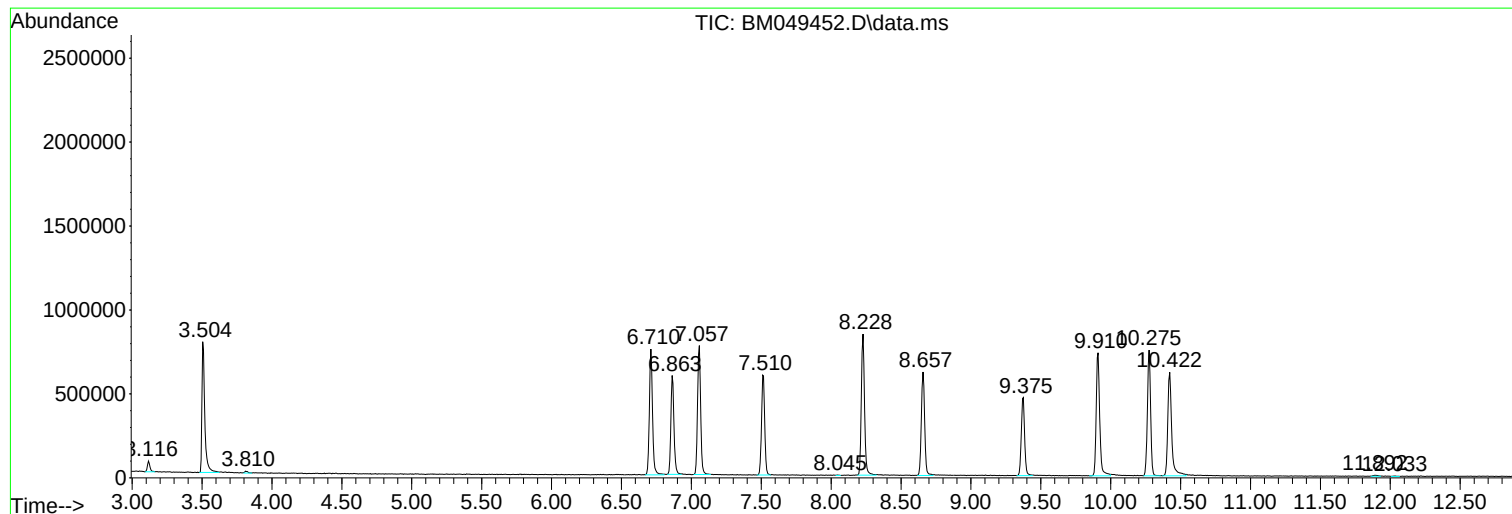

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049452.D
Acq On : 27 Jan 2025 17:23
Operator : RC/JU
Sample : PB166251BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012725\
Data File : BM049452.D
Acq On : 27 Jan 2025 17:23
Operator : RC/JU
Sample : PB166251BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc