

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000376.D
 Acq On : 29 Jan 2015 05:59
 Operator : TP/IZ
 Sample : G1134-07RX
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA5RX

Quant Time: Jan 29 14:52:47 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 06:48:28 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	164845	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	665318	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	414232	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	964942	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	1060396	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	980646	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	5060	1.97	ng/uL	0.00
5) Phenol-d5	6.90	99	86656	8.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	140039	20.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	161591	18.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	120800	14.99	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	75331	19.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	77801	21.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	174620	19.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	5685	0.50	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	722797	26.28	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	796965	22.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.58	143	27694	7.29	ng/ul	0.00
57) Fluorene-d10	15.38	176	617749	23.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	72065	18.08	ng/ul	0.00
70) Anthracene-d10	17.23	188	1003815	22.74	ng/ul	0.00
76) Pyrene-d10	19.53	212	1184073	24.18	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1063343	23.73	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.79	165	6327	1.41	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
Data File : BM000376.D
Acq On : 29 Jan 2015 05:59
Operator : TP/IZ
Sample : G1134-07RX
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA5RX

Quant Time: Jan 29 14:52:47 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 29 06:48:28 2015
Response via : Initial Calibration

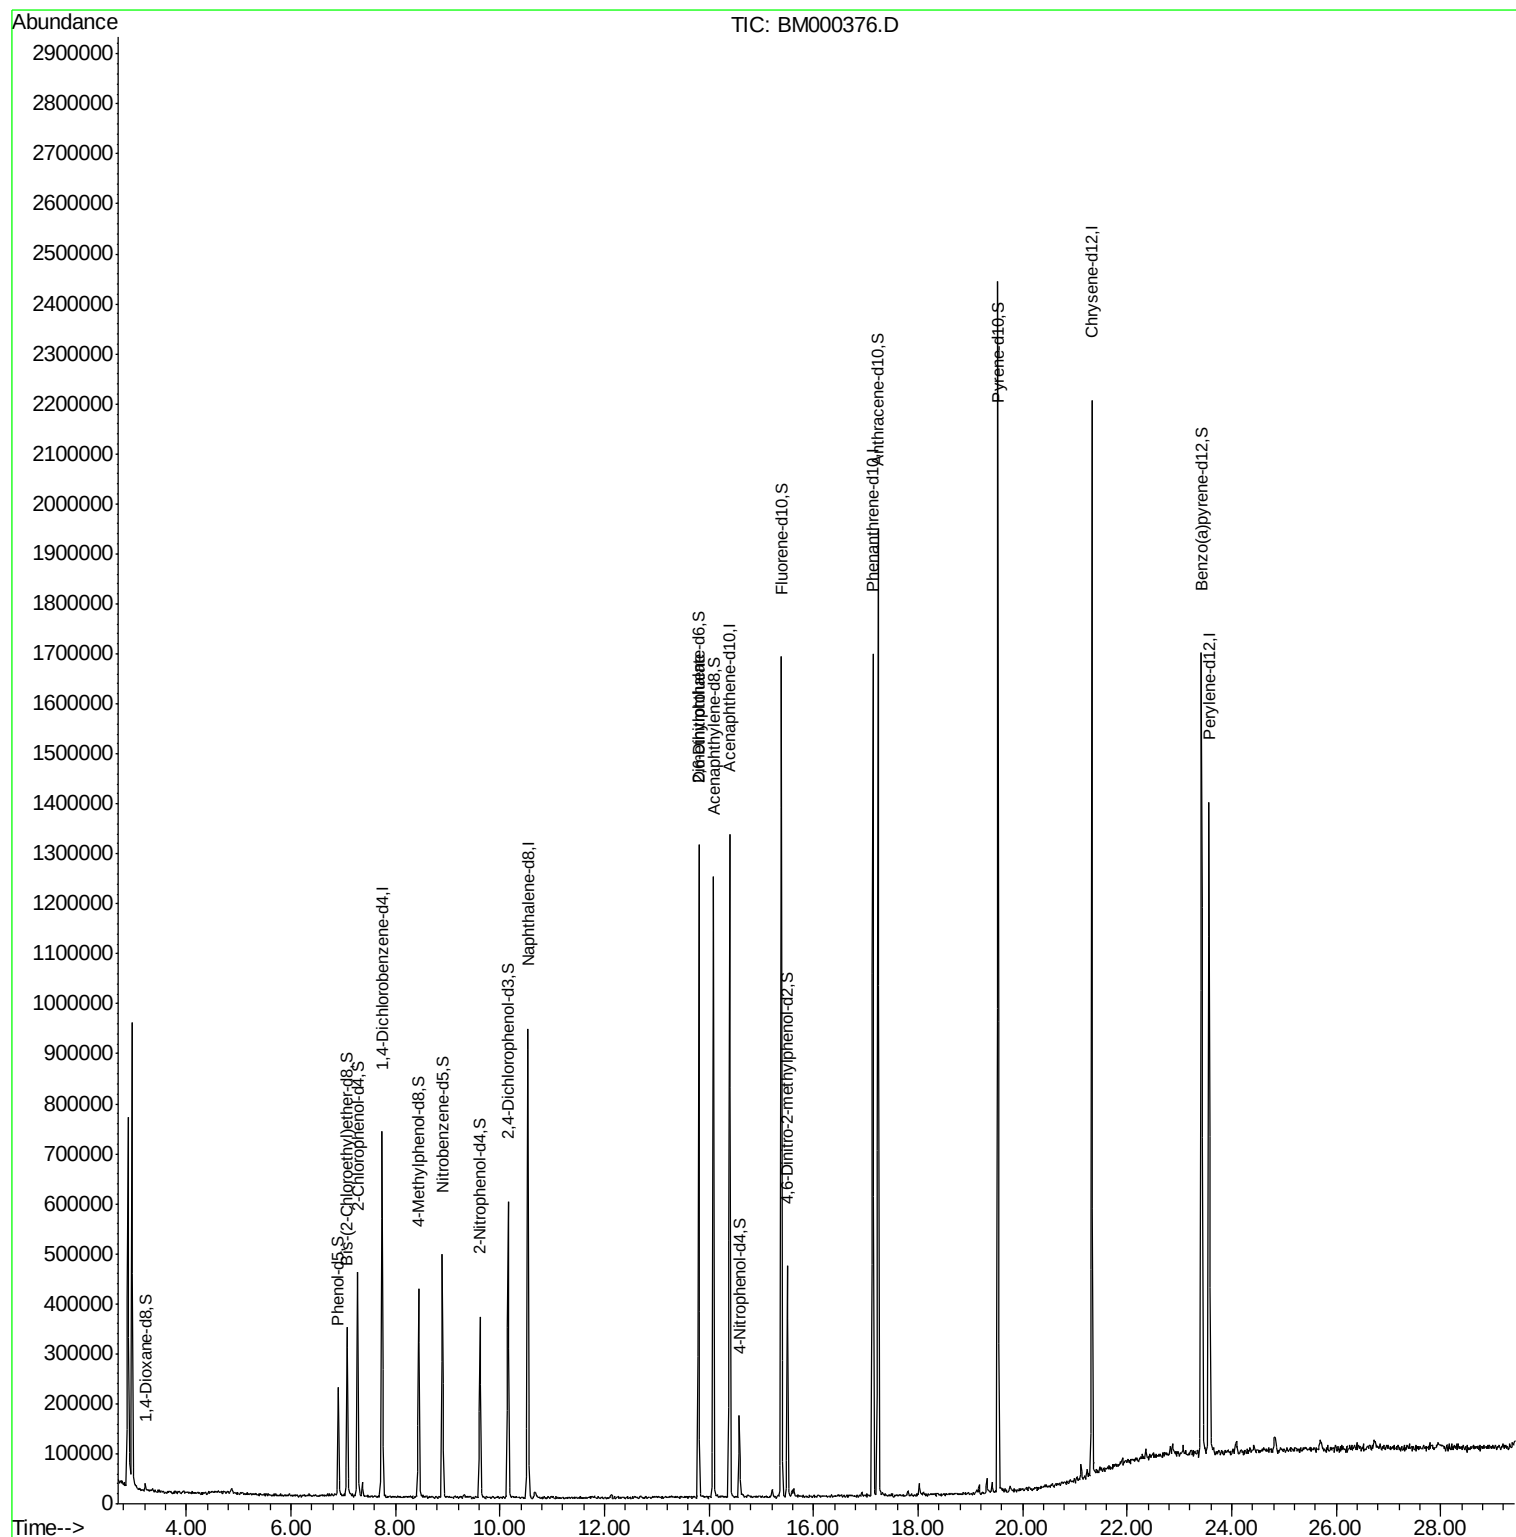

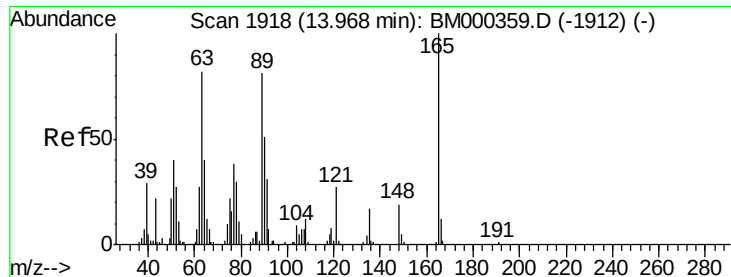

#45

2,6-Dinitrotoluene

Concen: 1.41 ng/ul

RT: 13.79 min Scan# 1888

Delta R.T. -0.18 min

Lab File: BM000376.D

Acq: 29 Jan 2015 05:59

Instrument :

BNA_M

ClientSampleId :

C0AA5RX



Tgt Ion:165 Resp: 6327

Ion Ratio Lower Upper

165 100

89 0.0 65.2 97.8#

121 33.5 21.5 32.3#

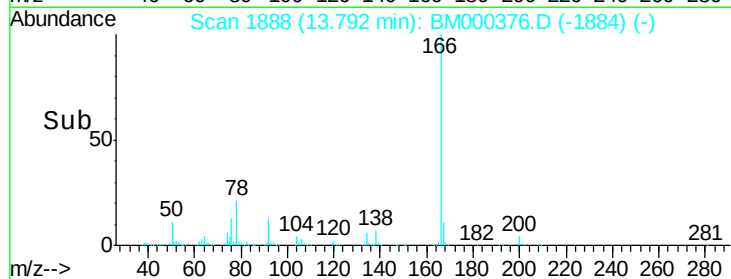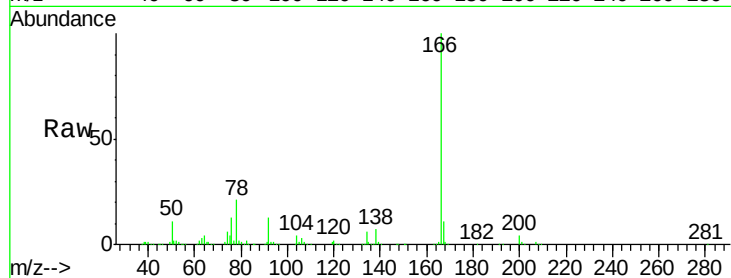

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

