

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000379.D
 Acq On : 29 Jan 2015 07:45
 Operator : TP/IZ
 Sample : G1134-10RX
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA9RX

Quant Time: Jan 29 14:53:05 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 06:48:28 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	147379	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	580497	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	367184	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	844815	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	921629	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	859863	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.21	96	1853	0.81	ng/uL	0.00
5) Phenol-d5	6.90	99	45139	4.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	138407	22.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	140478	18.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	82996	11.52	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	74402	22.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	77362	24.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	171472	21.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	9201	0.94	ng/ul	0.00
43) Dimethylphthalate-d6	13.79	166	655470	26.89	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	780053	24.85	ng/ul	0.00
51) 4-Nitrophenol-d4	14.58	143	11692	3.47	ng/ul	0.00
57) Fluorene-d10	15.38	176	588791	25.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	59936	17.17	ng/ul	0.00
70) Anthracene-d10	17.23	188	917267	23.73	ng/ul	0.00
76) Pyrene-d10	19.53	212	1039649	24.43	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	847503	21.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.80	165	6326	1.59	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
Data File : BM000379.D
Acq On : 29 Jan 2015 07:45
Operator : TP/IZ
Sample : G1134-10RX
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA9RX

Quant Time: Jan 29 14:53:05 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 29 06:48:28 2015
Response via : Initial Calibration

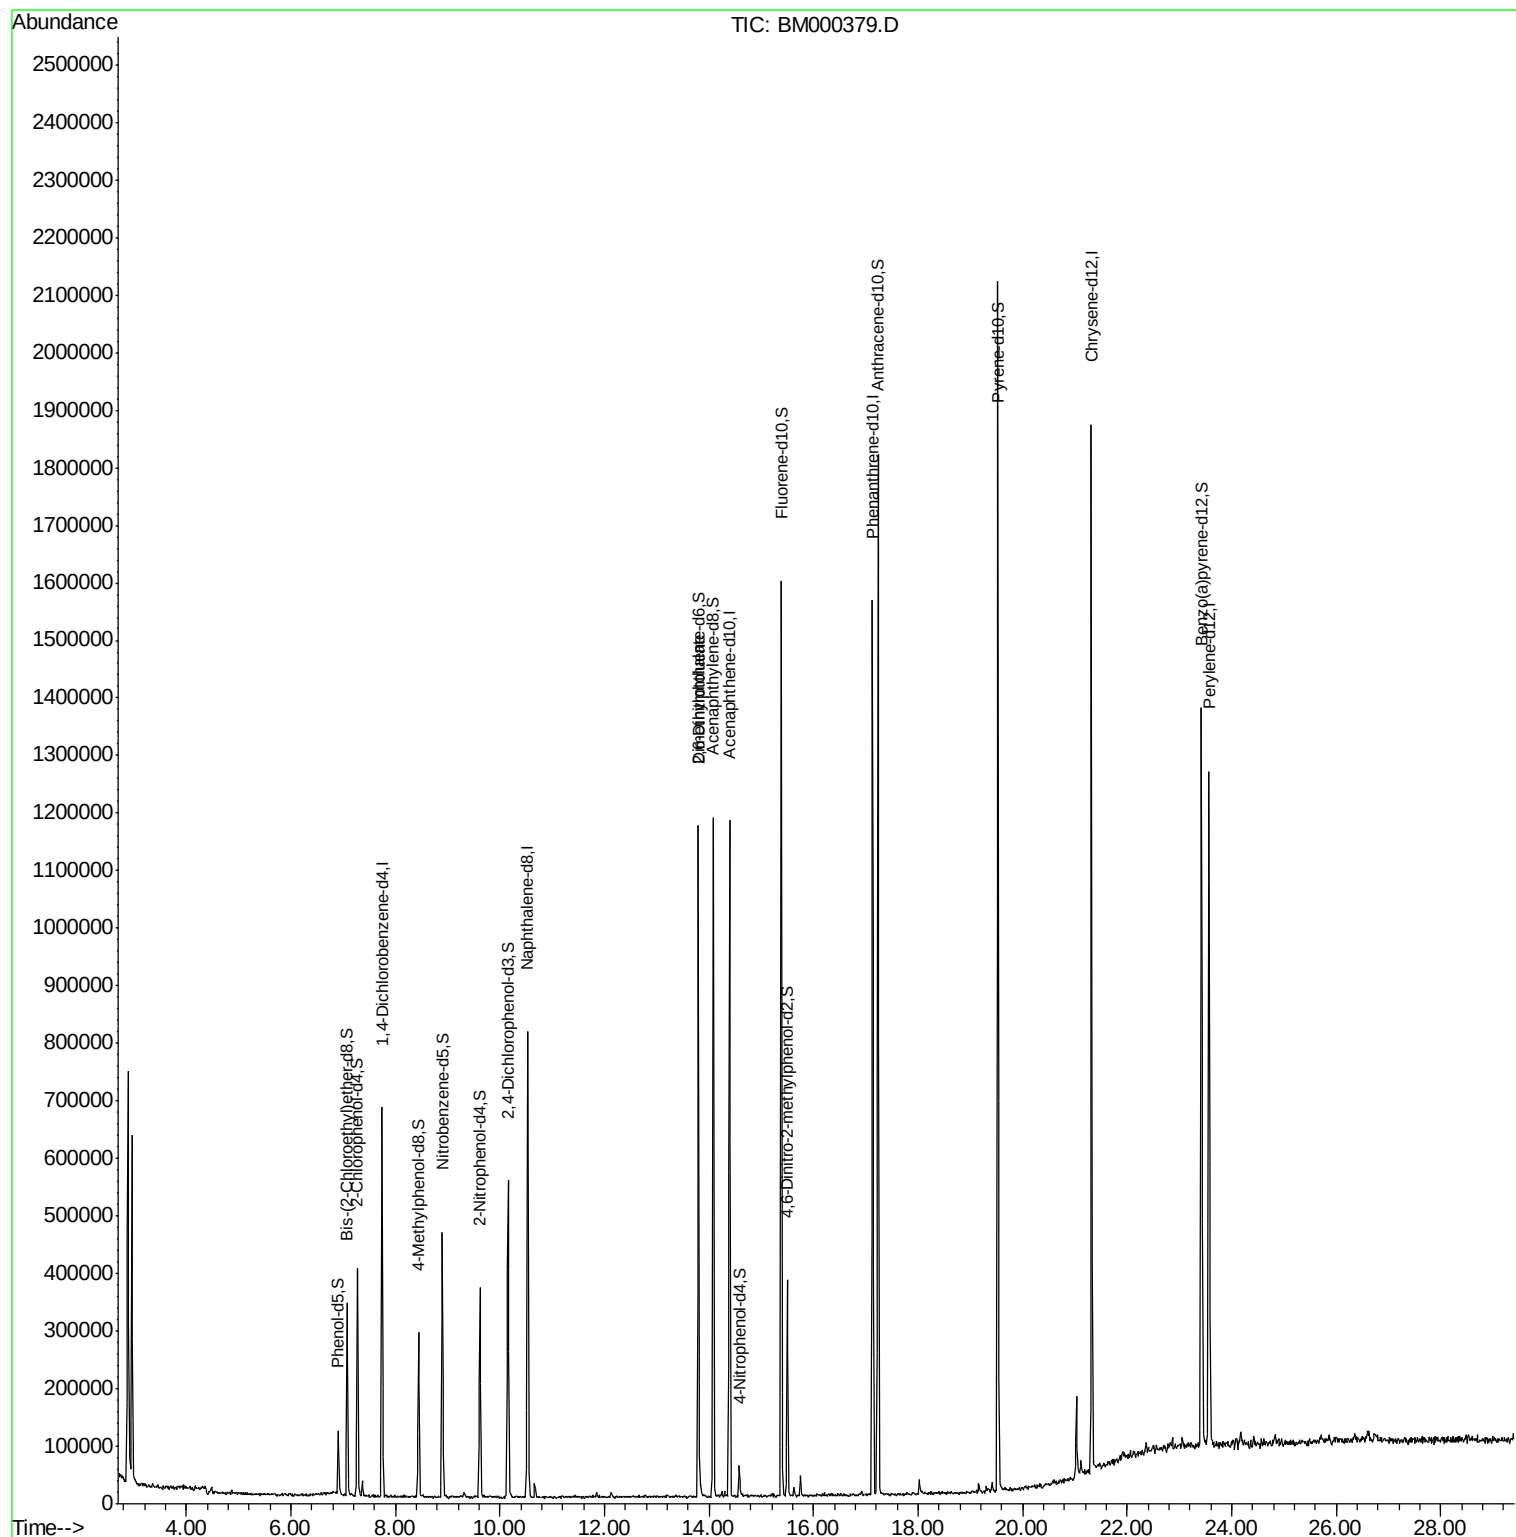

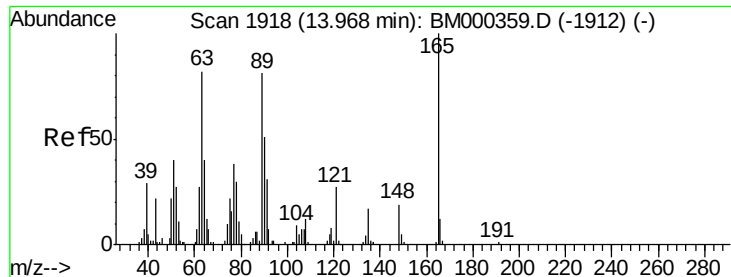

#45

2,6-Dinitrotoluene

Concen: 1.59 ng/ul

RT: 13.80 min Scan# 1889

Delta R.T. -0.17 min

Lab File: BM000379.D


Acq: 29 Jan 2015 07:45

Instrument :

BNA_M

ClientSampleId :

C0AA9RX

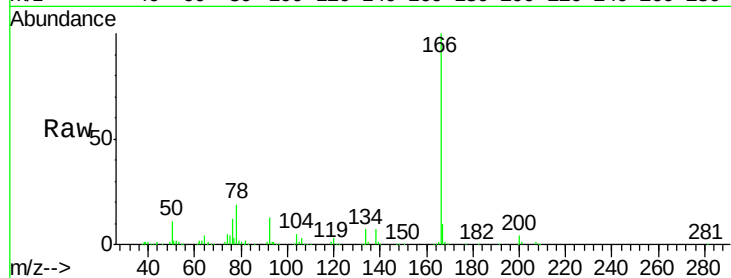

Tgt Ion:	165	Resp:	6326
Ion	Ratio	Lower	Upper
165	100		
89	0.0	65.2	97.8#
121	18.5	21.5	32.3#

