

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000380.D
 Acq On : 29 Jan 2015 08:20
 Operator : TP/IZ
 Sample : G1134-11RX
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB0RX

Quant Time: Jan 29 14:53:11 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 06:48:28 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	134350	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	539347	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	343823	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	816111	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	892676	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	827752	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	2290	1.10	ng/uL	0.00
5) Phenol-d5	6.90	99	36099	4.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	101580	17.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	109547	15.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	69425	10.57	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	57519	18.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	60075	20.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	142702	19.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	8083	0.88	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	572645	25.09	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	672052	22.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.58	143	11418	3.62	ng/ul	0.00
57) Fluorene-d10	15.38	176	510122	23.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	59252	17.57	ng/ul	0.00
70) Anthracene-d10	17.23	188	815558	21.84	ng/ul	0.00
76) Pyrene-d10	19.53	212	957838	23.24	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	798665	21.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.80	165	5017	1.35	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
Data File : BM000380.D
Acq On : 29 Jan 2015 08:20
Operator : TP/IZ
Sample : G1134-11RX
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB0RX

Quant Time: Jan 29 14:53:11 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 29 06:48:28 2015
Response via : Initial Calibration

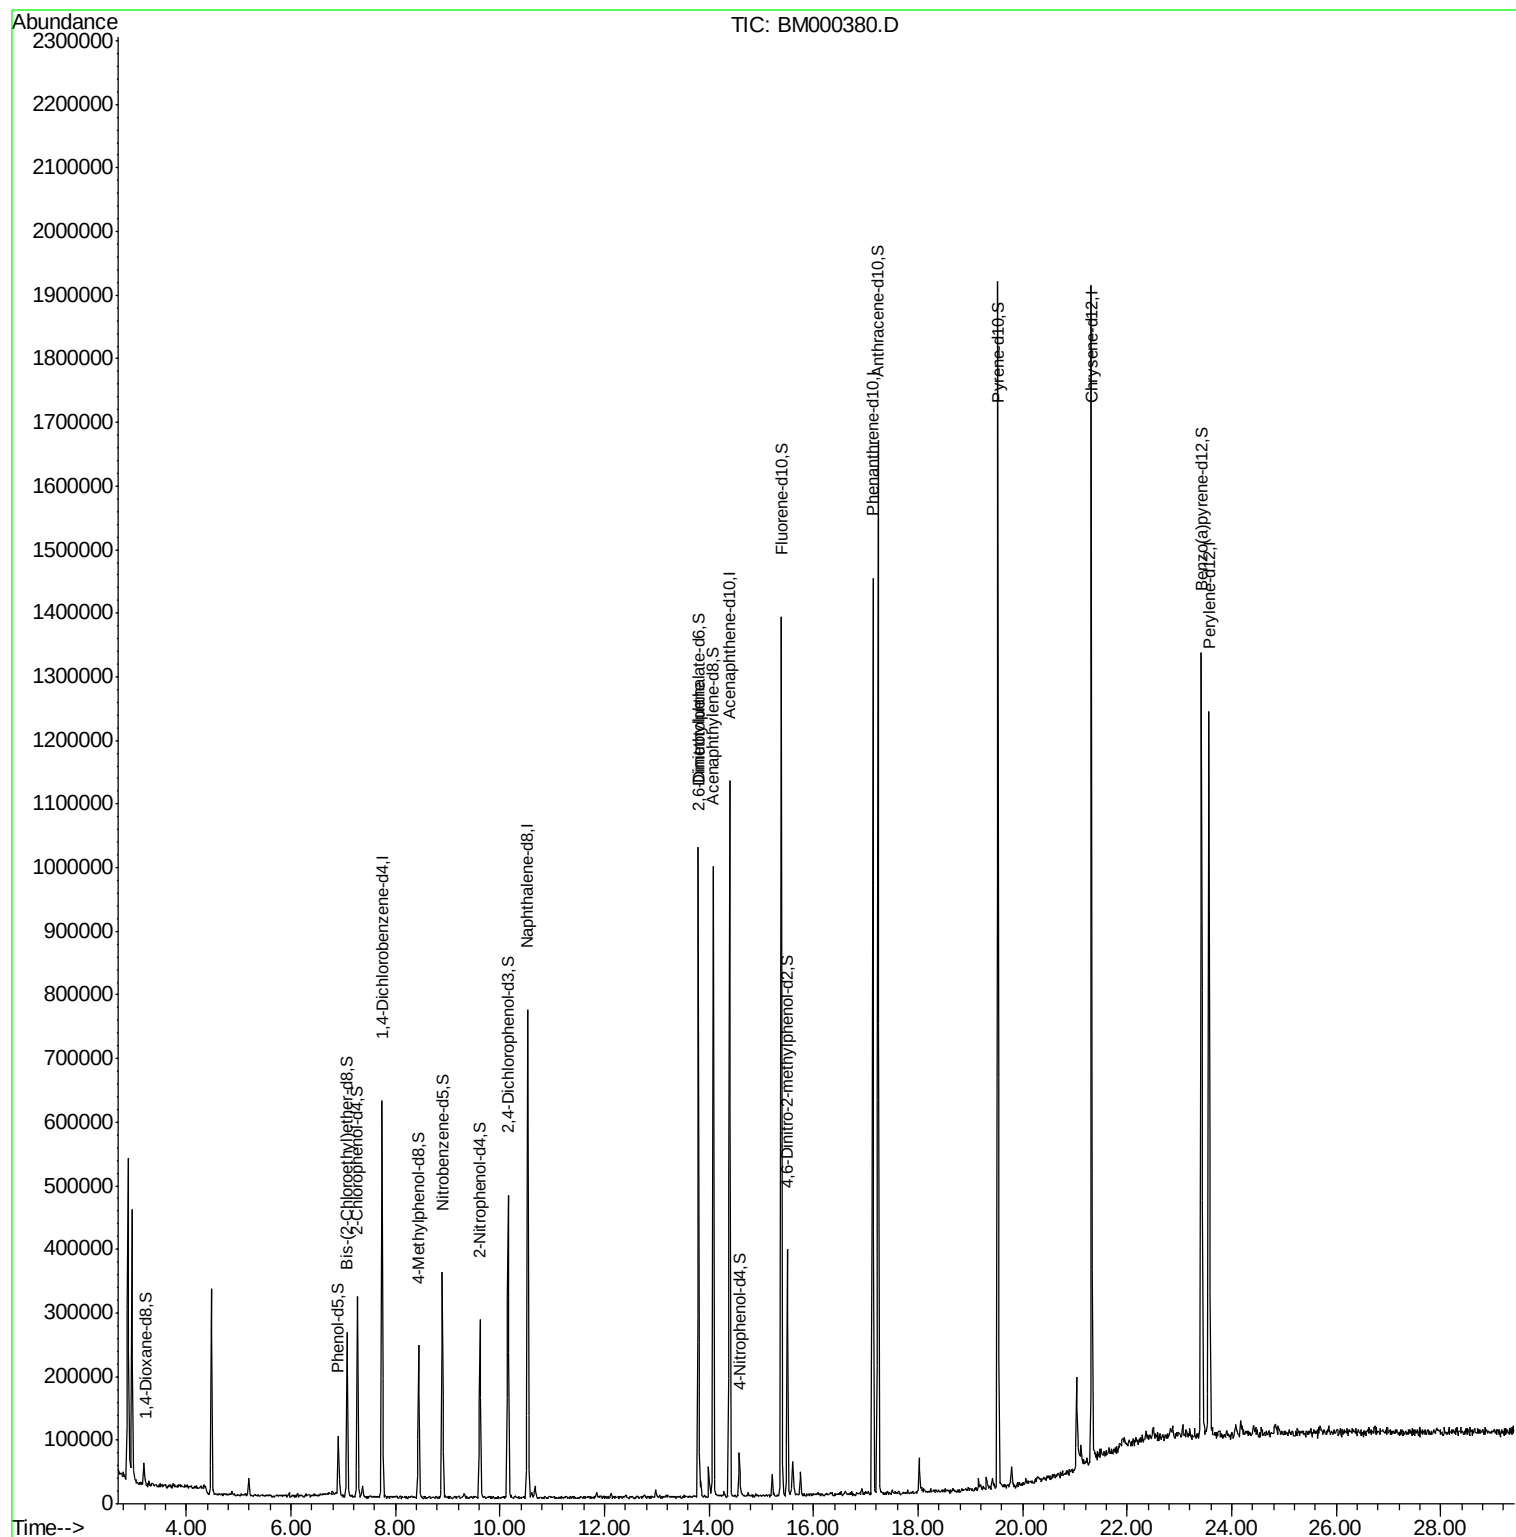

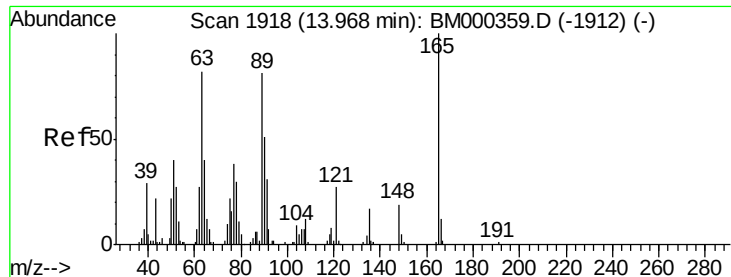

#45
 2,6-Dinitrotoluene
 Concen: 1.35 ng/ul
 RT: 13.80 min Scan# 1890
 Delta R.T. -0.16 min
 Lab File: BM000380.D
 Acq: 29 Jan 2015 08:20

Instrument :
 BNA_M
 ClientSampleId :
 C0AB0RX

Tgt Ion:165 Resp: 5017
 Ion Ratio Lower Upper
 165 100
 89 0.0 65.2 97.8#
 121 35.7 21.5 32.3#

