


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
Data File : BM000356.D
Acq On : 28 Jan 2015 16:52
Operator : TP/IZ
Sample : DFTPP12
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP12

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
Title : SVOA CALIBRATION
Last Update : Thu Jan 29 06:48:28 2015

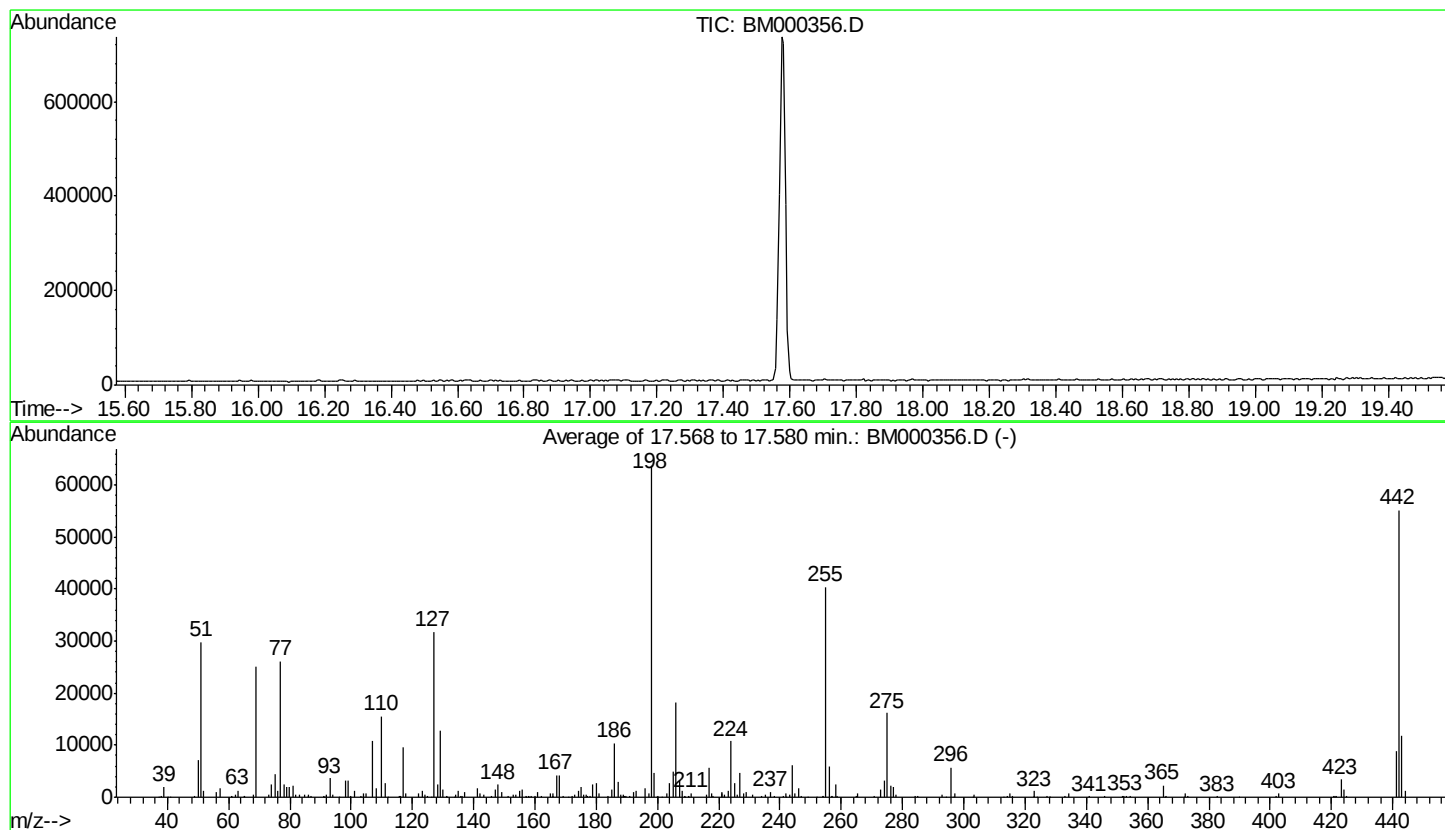

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2525

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	29874	PASS
68	69	0.00	2	1.7	416	PASS
69	198	0.00	100	39.5	25133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	31797	PASS
197	198	0.00	2	1.0	651	PASS
198	198	100	100	100.0	63690	PASS
199	198	5	9	7.3	4662	PASS
275	198	10	60	25.4	16204	PASS
365	198	1	100	3.6	2310	PASS
441	443	0.01	100	74.2	8739	PASS
442	198	50	100	86.6	55152	PASS
443	442	15	24	21.4	11781	PASS