

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000368.D
 Acq On : 29 Jan 2015 00:41
 Operator : TP/LZ
 Sample : G1115-13RX
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 COAW1RX

Manual Integrations
 APPROVED

apatel
 2/5/2015 12:07:48 PM

Quant Time: Jan 29 15:50:02 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 15:21:44 2015
 Response via : Initial Calibration

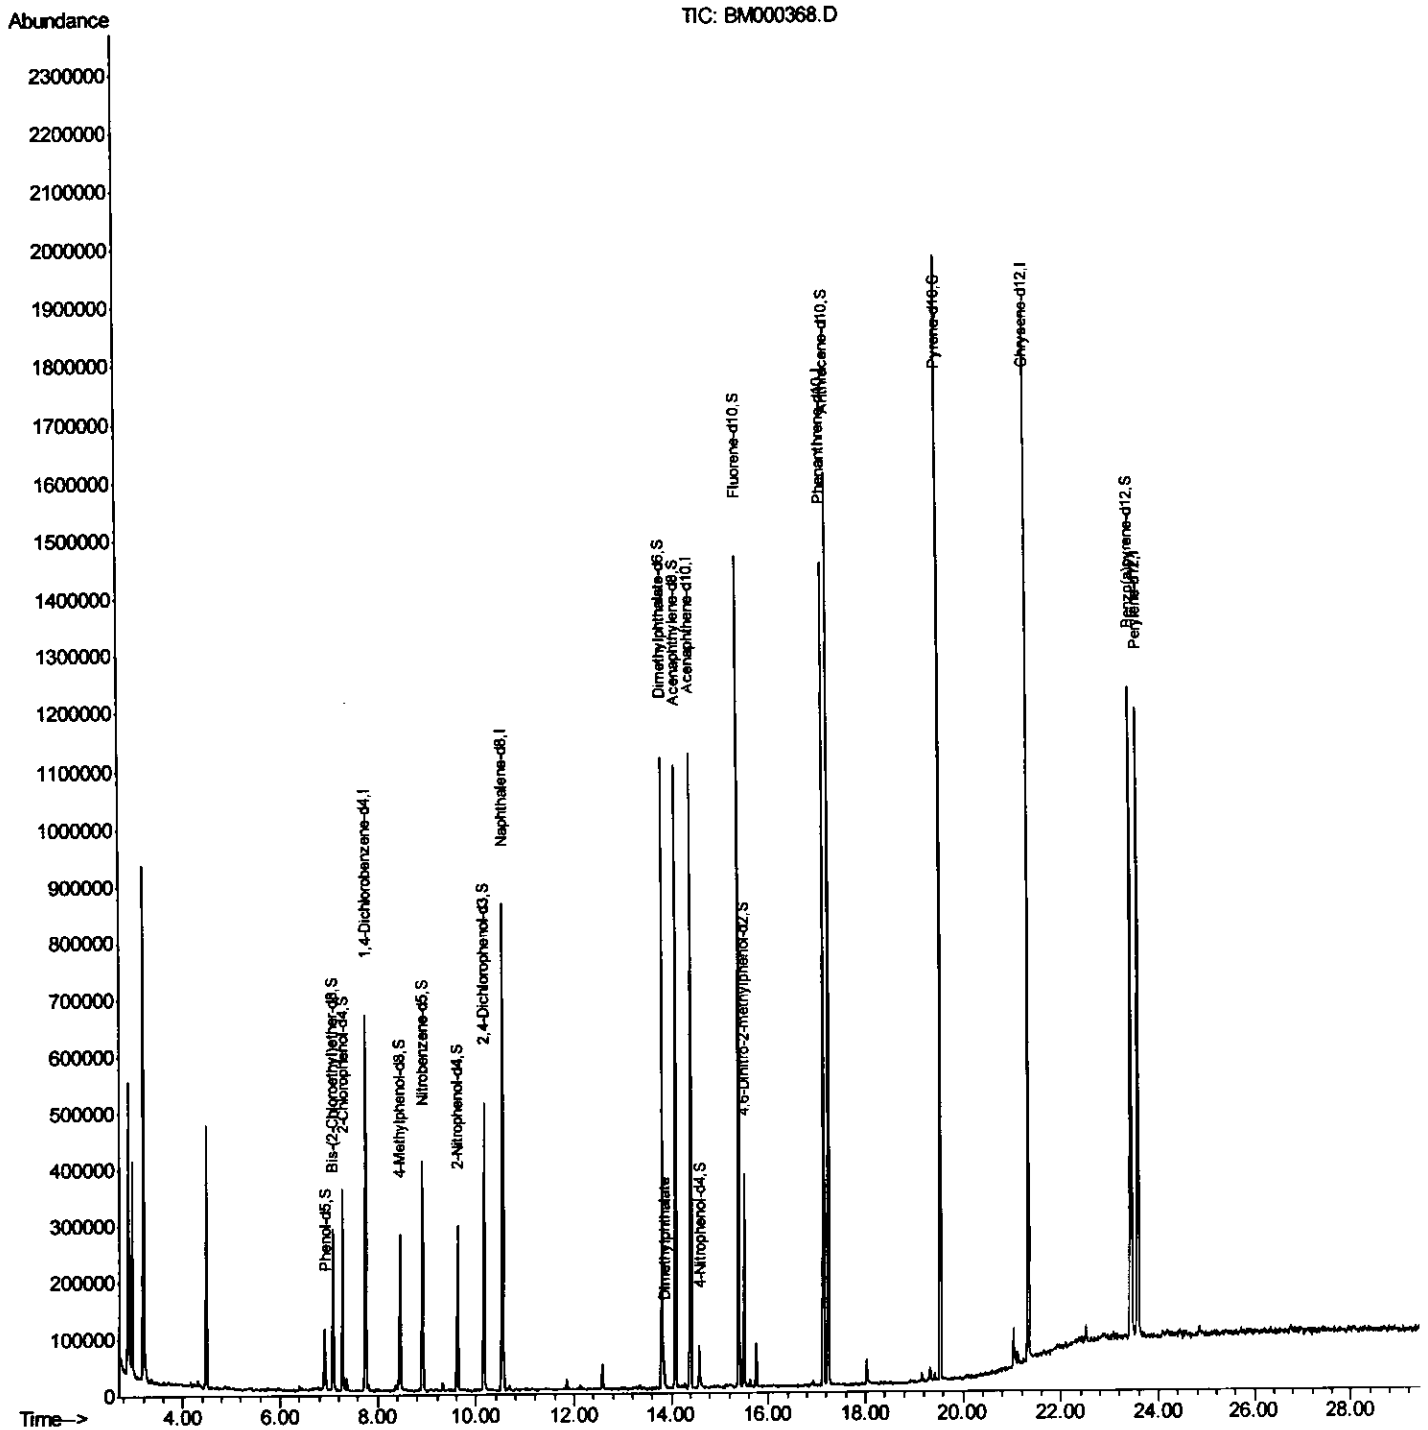

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000368.D
 Acq On : 29 Jan 2015 00:41
 Operator : TP/IZ
 Sample : G1115-13RX
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW1RX

Quant Time: Jan 29 15:37:08 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 15:21:44 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 2/5/2015 12:07:48 PM

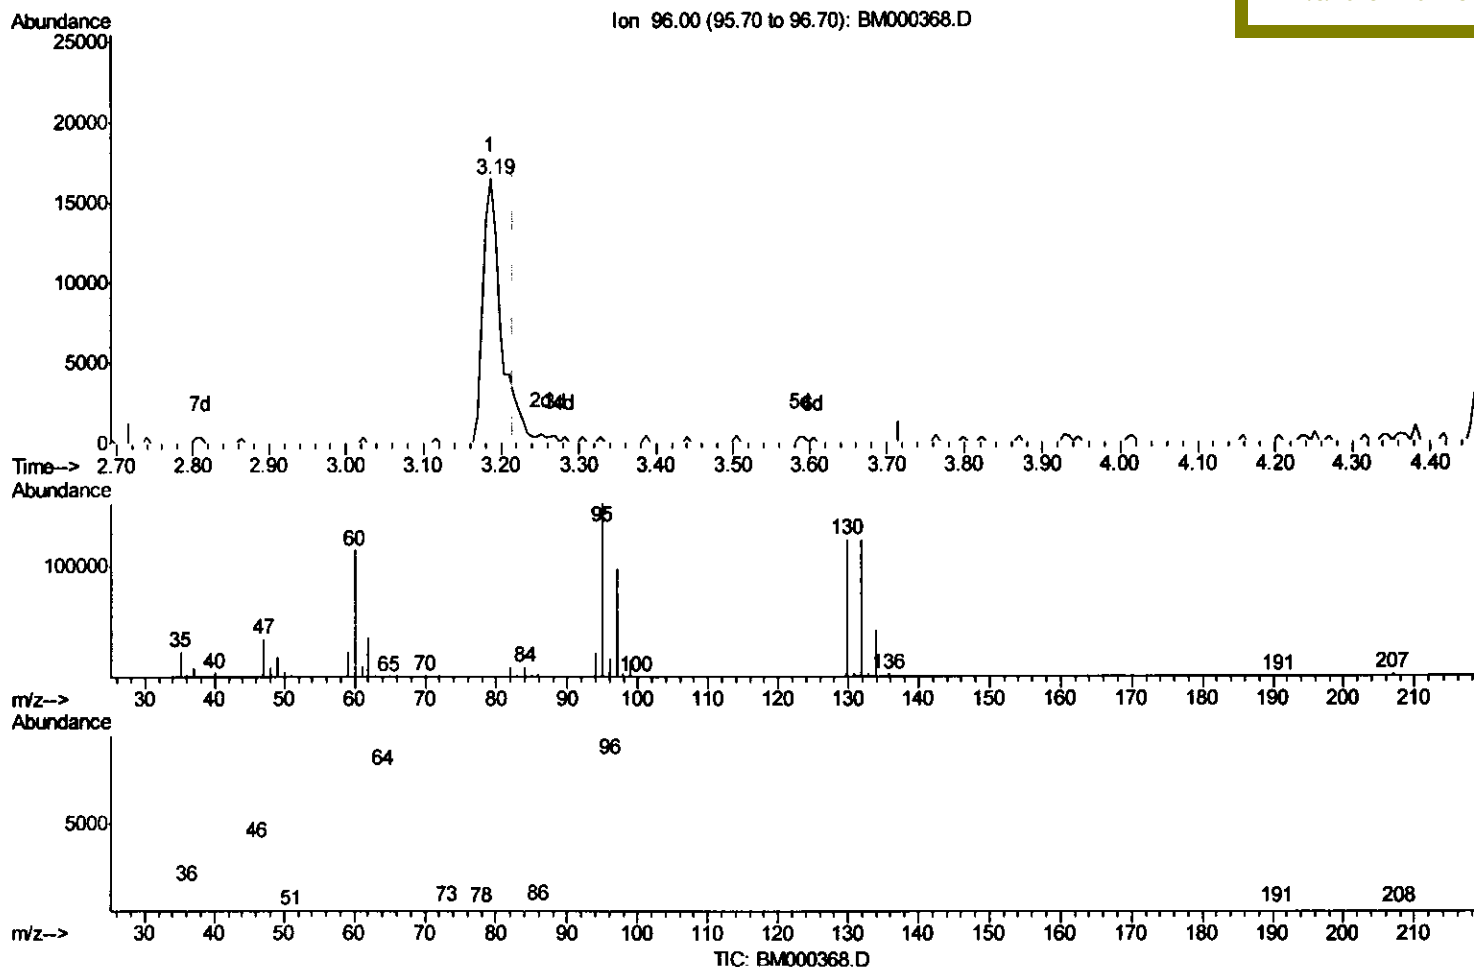

(3) 1,4-Dioxane-d8 (S)

3.187min (-0.029) 11.32ng/uL

response 26256

Ion	Exp%	Act%
96.00	100	100
64.00	20.00	0.00#
34.00	20.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000368.D
 Acq On : 29 Jan 2015 00:41
 Operator : TP/I2
 Sample : G1115-13RX
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAW1RX

Manual Integrations
 APPROVED

apatel
 2/5/2015 12:07:48 PM

Quant Time: Jan 29 15:37:08 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 15:21:44 2015
 Response via : Initial Calibration

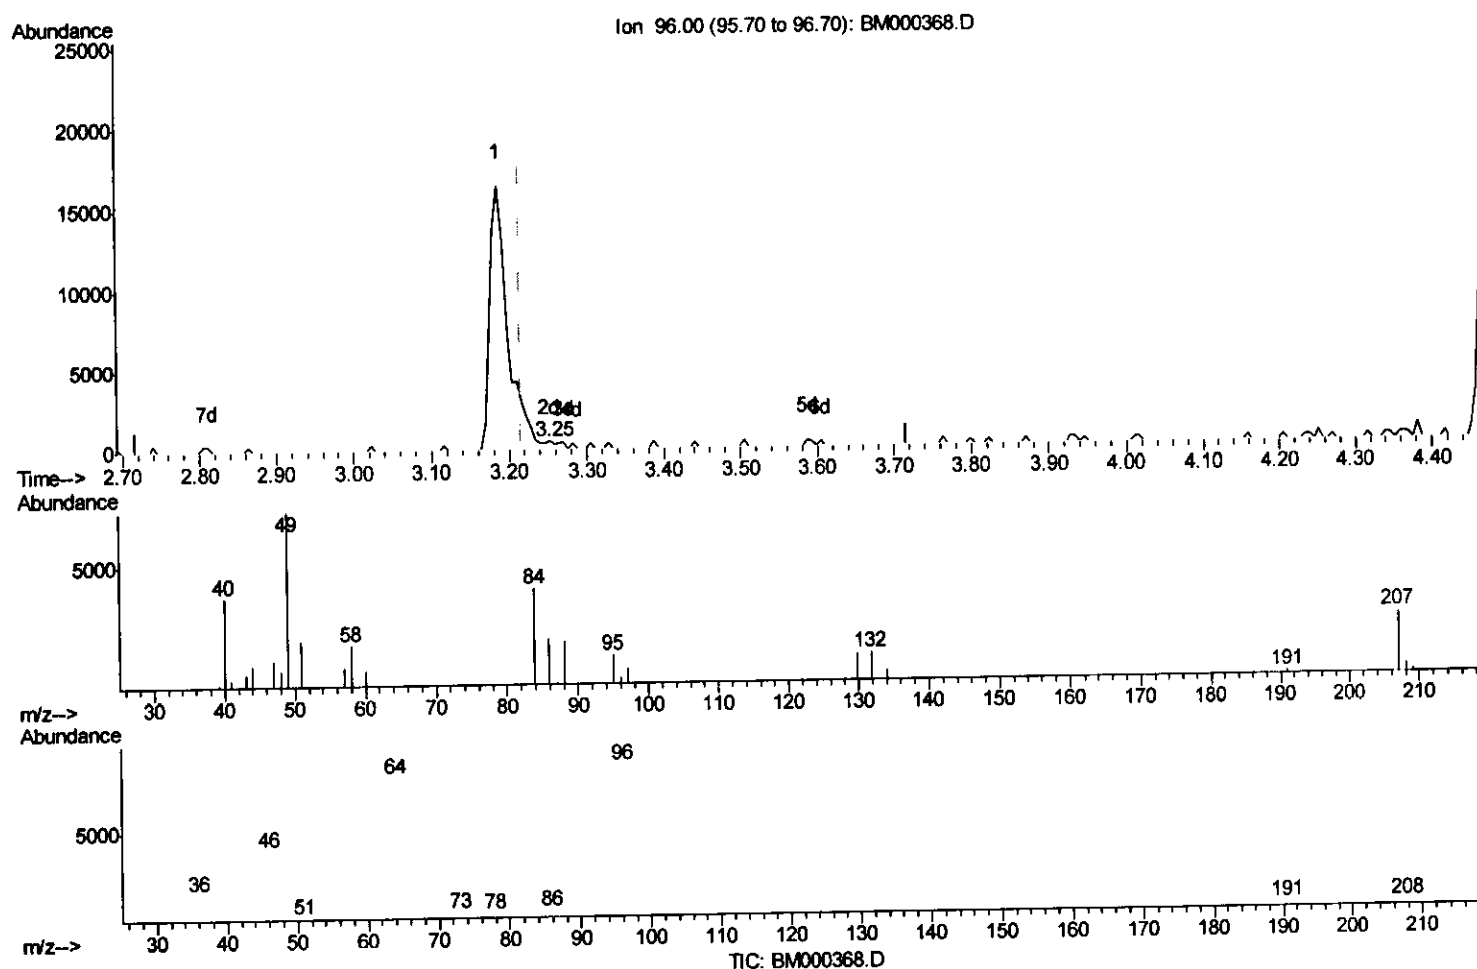

(3) 1,4-Dioxane-d8 (S)

3.252min (+0.035) 0.30ng/uL m

response 704

Ion	Exp%	Act%
96.00	100	100
64.00	20.00	0.00#
34.00	20.00	0.00#
0.00	0.00	0.00

T.P.
 2/5/15

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
 Data File : BM000368.D
 Acq On : 29 Jan 2015 00:41
 Operator : TP/IZ
 Sample : G1115-13RX
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAW1RX

Quant Time: Jan 29 15:50:02 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 29 15:21:44 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 2/5/2015 12:07:48 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	149219	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	581049	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	353577	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	799141	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	857014	20.00	ng/ul	0.00
83) Perylene-d12	23.57	264	816572	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	704m	0.30	ng/uL	0.04
5) Phenol-d5	6.91	99	45437	4.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	120003	19.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	128304	16.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	80851	11.08	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	62617	18.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	64408	20.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	149863	18.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	3550	0.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	606773	25.85	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	700165	23.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.58	143	12990	4.01	ng/ul	0.00
57) Fluorene-d10	15.38	176	540167	24.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	59677	18.07	ng/ul	0.00
70) Anthracene-d10	17.23	188	834191	22.82	ng/ul	0.00
76) Pyrene-d10	19.53	212	981258	24.80	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	779781	20.90	ng/ul	0.00

TP.
 2/5/15

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.84	163	28025	1.16	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed