


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012815\
Data File : BM000356.D
Acq On : 28 Jan 2015 16:52
Operator : TP/IZ
Sample : DFTPP12
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP12

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012815.M
Title : SVOA CALIBRATION
Last Update : Thu Jan 29 15:49:59 2015

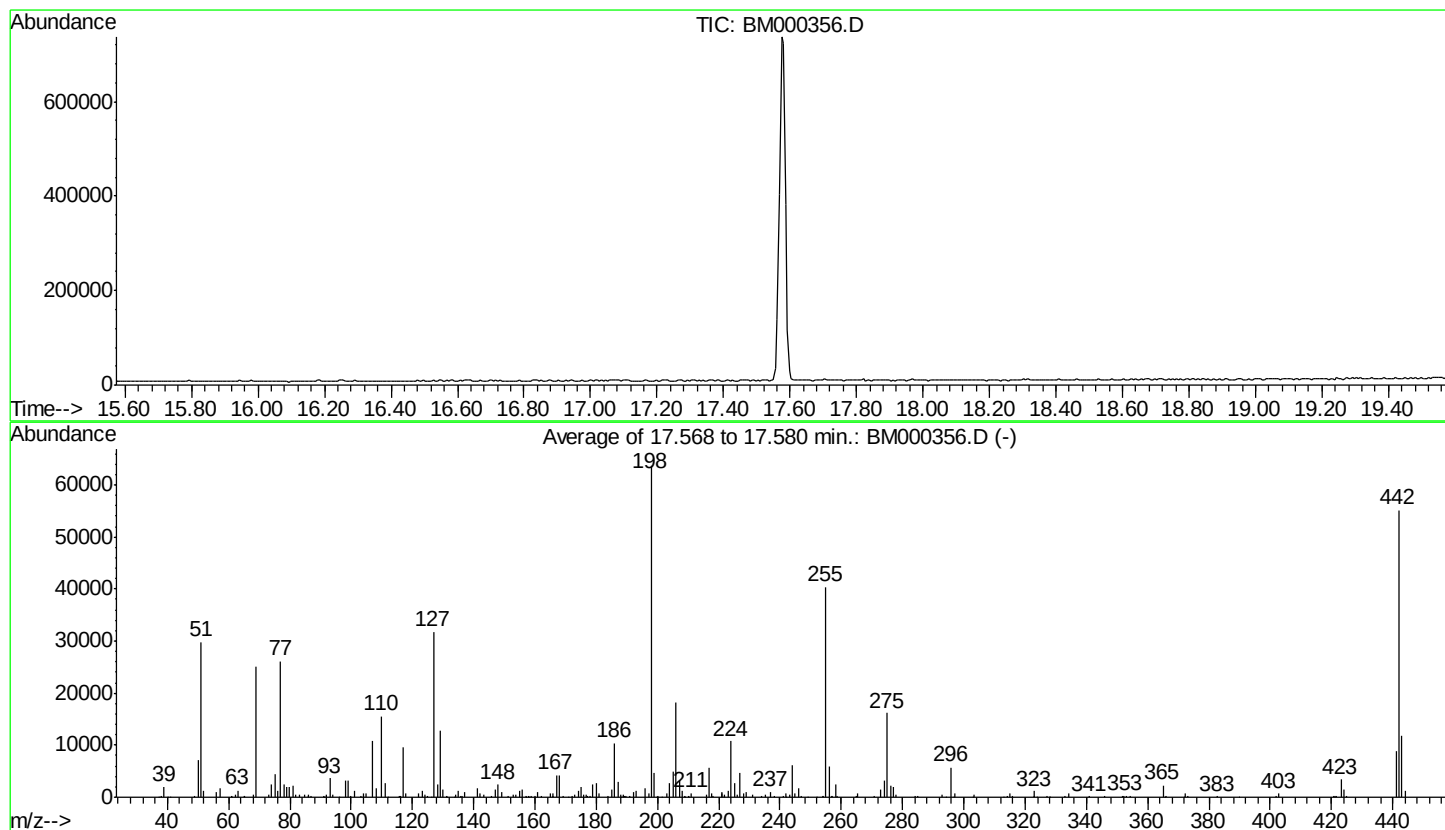

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2525

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	29874	PASS
68	69	0.00	2	1.7	416	PASS
69	198	0.00	100	39.5	25133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	31797	PASS
197	198	0.00	2	1.0	651	PASS
198	198	100	100	100.0	63690	PASS
199	198	5	9	7.3	4662	PASS
275	198	10	60	25.4	16204	PASS
365	198	1	100	3.6	2310	PASS
441	443	0.01	100	74.2	8739	PASS
442	198	50	100	86.6	55152	PASS
443	442	15	24	21.4	11781	PASS

m/z	Abundance
39.10	1920.0
40.00	5013.0
44.00	3803.0
50.10	5458.0
51.10	22096.0
51.90	738.0
55.90	891.0
57.00	1086.0
60.90	312.0
62.10	334.0
63.00	977.0
67.90	328.0
69.00	18344.0
73.00	384.0
74.10	2276.0
75.00	3690.0
76.00	1254.0
77.10	17128.0
78.10	2125.0
79.20	1324.0
80.00	1420.0
81.00	1798.0
82.10	452.0
83.10	319.0
85.90	741.0
90.90	329.0
91.90	666.0
93.00	3812.0
93.90	553.0
98.00	2444.0
99.00	2921.0
101.00	1035.0
103.10	644.0
103.90	763.0
105.00	717.0
107.00	8030.0
108.10	1226.0
110.10	10360.0
111.00	1842.0
116.20	307.0
117.00	6280.0
118.00	340.0
122.00	496.0
123.10	639.0
124.00	440.0
127.00	22536.0
128.10	2408.0
129.00	10788.0
130.00	1427.0
134.10	372.0
135.00	909.0
135.90	543.0
137.00	781.0
141.00	1156.0
142.00	310.0
143.10	609.0
145.90	441.0
147.10	1284.0
148.00	1665.0
149.00	818.0
155.00	887.0
156.00	1032.0
157.20	372.0
157.80	460.0
161.10	759.0
167.00	2468.0
168.00	4192.0
169.10	641.0
170.90	332.0
173.10	394.0
174.10	1294.0
175.00	1277.0
176.00	387.0
176.70	372.0
177.90	377.0
178.90	1632.0
180.00	1658.0
181.10	440.0
185.00	1222.0
186.10	6781.0
187.00	2056.0
188.00	473.0
188.80	715.0
192.00	885.0
193.10	727.0
196.00	1152.0
198.00	39656.0
199.00	3252.0
200.10	535.0
201.50	380.0
203.10	555.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

203.90	1449.0
205.10	3658.0
206.10	12140.0
207.10	2845.0
208.10	886.0
210.90	337.0
216.00	476.0
217.00	3525.0
217.80	304.0
221.10	1311.0
221.70	728.0
223.10	595.0
224.10	6817.0
225.10	1892.0
226.10	303.0
227.00	3272.0
228.00	604.0
229.20	334.0
231.10	481.0
235.20	424.0
237.00	840.0
237.90	314.0
241.80	305.0
243.00	506.0
244.10	3866.0
245.00	322.0
246.00	1726.0
255.00	22168.0
256.00	2858.0
257.90	1228.0
264.90	725.0
272.90	845.0
274.00	2550.0
275.00	8429.0
276.10	1348.0
277.00	1119.0
278.00	534.0
292.90	401.0
294.00	334.0
296.00	3598.0
296.70	382.0
302.90	306.0
315.00	541.0
322.90	803.0
323.90	311.0
334.10	344.0
352.20	348.0
364.90	1132.0
365.70	362.0
371.80	338.0
373.10	339.0
402.80	359.0
423.00	1388.0
424.00	1250.0
425.00	368.0
441.00	4491.0
442.00	27064.0
443.00	5777.0
443.90	712.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

m/z	Abundance
37.00	309.0
37.90	460.0
39.00	2071.0
40.00	4402.0
41.10	318.0
44.10	3442.0
50.10	9307.0
51.10	37704.0
52.00	1745.0
55.90	1380.0
57.10	2165.0
61.10	1005.0
62.10	695.0
63.00	1300.0
65.00	607.0
68.00	605.0
69.00	31520.0
72.90	496.0
74.00	3606.0
75.00	5196.0
76.10	1820.0
77.10	31904.0
78.00	3341.0
79.00	2897.0
80.00	2370.0
81.10	2509.0
82.10	710.0
83.10	559.0
85.00	677.0
86.10	821.0
86.90	707.0
91.10	541.0
92.10	492.0
93.10	3675.0
94.00	493.0
96.00	303.0
98.00	3823.0
99.00	3902.0
101.10	1270.0
103.10	341.0
104.10	1163.0
104.90	664.0
107.00	11768.0
108.00	2077.0
110.00	19560.0
111.00	2949.0
116.10	777.0
117.10	11774.0
117.90	774.0
122.10	1052.0
123.10	1600.0
124.10	453.0
125.00	418.0
126.20	342.0
127.00	39200.0
128.00	2768.0
129.00	14568.0
130.00	1724.0
131.00	343.0
133.70	382.0
134.10	499.0
134.90	1421.0
136.10	475.0
137.00	1307.0
141.00	1792.0
141.90	759.0
143.10	746.0
146.90	1361.0
148.00	2844.0
149.00	1135.0
152.90	941.0
153.90	622.0
155.00	1309.0
156.00	1442.0
156.90	333.0
158.00	347.0
158.90	306.0
159.90	694.0
160.90	1295.0
161.90	469.0
165.00	1114.0
165.70	539.0
166.20	536.0
167.00	6061.0
168.10	4951.0
169.00	339.0
172.00	473.0
172.90	721.0
174.00	1286.0
175.10	2553.0
176.00	594.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

176.80	851.0
178.00	431.0
178.90	2546.0
180.10	3227.0
180.90	968.0
184.00	566.0
185.00	1570.0
186.00	12284.0
187.10	3903.0
188.10	591.0
188.70	552.0
189.10	766.0
191.00	368.0
191.90	1076.0
193.00	1328.0
196.10	2292.0
197.10	1194.0
198.00	76776.0
199.00	5167.0
200.00	576.0
202.90	423.0
204.00	3070.0
205.10	4583.0
206.00	21432.0
207.10	4992.0
208.00	1541.0
208.90	516.0
210.00	535.0
211.00	1157.0
216.10	753.0
217.00	6455.0
217.80	579.0
218.10	608.0
220.90	1156.0
221.80	910.0
222.90	1057.0
224.00	13112.0
225.10	3353.0
226.10	733.0
226.90	6041.0
228.10	1245.0
229.00	1035.0
231.10	522.0
234.00	503.0
235.10	556.0
236.90	1010.0
238.00	416.0
240.90	331.0
242.10	1020.0
243.00	640.0
244.10	7097.0
244.90	807.0
246.10	1326.0
247.00	492.0
249.10	310.0
254.20	737.0
255.00	50080.0
256.00	8365.0
256.90	629.0
258.00	2299.0
258.80	470.0
265.10	936.0
272.80	2017.0
274.00	3078.0
275.00	18096.0
276.10	2611.0
276.90	1744.0
278.00	463.0
292.90	674.0
296.00	5770.0
296.90	923.0
303.20	803.0
314.00	431.0
315.00	974.0
316.00	540.0
323.10	2045.0
327.20	402.0
327.80	374.0
332.90	510.0
334.10	955.0
341.10	500.0
352.20	515.0
353.10	427.0
354.20	556.0
365.00	3374.0
366.20	320.0
372.10	1114.0
373.10	411.0
382.90	428.0
389.90	375.0
402.00	638.0
402.90	814.0
420.90	443.0
421.90	323.0
423.00	3928.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

424.00	1429.0
424.80	351.0
441.00	9167.0
442.00	58480.0
443.10	13757.0
443.90	1184.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

m/z	Abundance
38.00	429.0
39.10	2168.0
40.00	4657.0
44.00	3748.0
48.80	407.0
50.00	6795.0
51.10	29824.0
52.10	1515.0
55.90	744.0
57.00	2137.0
62.00	812.0
63.00	1495.0
65.20	519.0
67.90	317.0
69.00	25536.0
72.90	568.0
74.00	1807.0
75.00	4495.0
76.00	956.0
77.00	29208.0
78.10	1954.0
78.90	1506.0
79.90	2278.0
81.00	2435.0
81.90	392.0
83.00	311.0
84.90	595.0
86.00	796.0
91.00	386.0
92.10	954.0
92.90	3319.0
94.10	417.0
98.00	3487.0
99.00	2629.0
99.90	650.0
101.10	1527.0
104.00	1315.0
104.90	968.0
107.10	12373.0
108.00	1862.0
110.00	16928.0
111.10	3251.0
112.00	331.0
115.90	725.0
117.00	10600.0
117.90	1049.0
122.10	638.0
123.00	1399.0
124.10	412.0
125.00	520.0
127.00	33656.0
128.10	2422.0
129.00	13293.0
129.90	1333.0
131.20	655.0
134.00	746.0
135.10	1115.0
136.00	525.0
137.10	1062.0
141.10	2493.0
142.10	991.0
143.00	413.0
145.90	425.0
147.00	1733.0
148.00	2665.0
149.00	818.0
151.20	436.0
152.80	714.0
153.90	553.0
155.10	1287.0
156.00	2150.0
157.10	371.0
157.70	311.0
159.00	382.0
159.80	382.0
160.90	912.0
161.90	435.0
165.00	809.0
166.00	1483.0
167.00	4094.0
168.00	3473.0
172.00	319.0
172.90	412.0
174.00	908.0
175.10	2002.0
176.10	300.0
177.00	629.0
179.00	3000.0
179.90	2914.0
181.10	795.0
183.90	327.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

185.10	2011.0
186.10	11973.0
187.00	3085.0
187.80	395.0
188.20	527.0
188.90	429.0
189.80	490.0
191.10	745.0
192.10	988.0
193.00	1867.0
195.90	1782.0
197.00	761.0
198.00	74640.0
199.10	5569.0
199.80	315.0
202.90	930.0
204.00	3360.0
205.00	6751.0
206.10	21336.0
207.10	3314.0
208.00	935.0
209.10	380.0
210.20	319.0
211.10	738.0
216.10	471.0
216.90	6964.0
217.90	1111.0
221.20	2803.0
222.00	598.0
223.00	1996.0
224.10	12393.0
225.20	2861.0
226.10	680.0
227.10	4867.0
228.10	739.0
228.90	1586.0
231.10	487.0
235.00	563.0
237.00	1236.0
238.00	315.0
240.90	328.0
242.10	859.0
243.00	699.0
244.10	7826.0
244.90	995.0
246.00	1968.0
246.90	592.0
252.10	388.0
253.90	535.0
255.00	48928.0
256.10	6424.0
257.10	675.0
258.00	3876.0
258.80	530.0
265.10	1174.0
270.90	402.0
273.00	1345.0
274.00	4118.0
275.00	22088.0
276.00	2361.0
277.00	2987.0
277.90	748.0
284.00	493.0
285.00	756.0
292.80	688.0
296.00	7754.0
297.00	1293.0
303.10	1047.0
312.90	315.0
314.10	366.0
315.00	924.0
323.00	1420.0
328.00	352.0
332.90	347.0
334.10	1311.0
346.10	581.0
351.90	571.0
352.90	588.0
354.10	347.0
365.00	2424.0
366.10	546.0
372.00	1251.0
403.00	992.0
420.70	367.0
421.20	529.0
421.70	730.0
423.10	4751.0
423.90	1597.0
425.00	361.0
441.00	12561.0
442.00	79912.0
443.10	15810.0
444.00	1765.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12

Scan 2525 (17.539 min): BM000356.D
DFTPP12

m/z	Abundance
40.00	4647.0
44.00	3830.0
206.90	594.0

Instrument :
BNA_M
ClientSampleId :
DFTPP12