
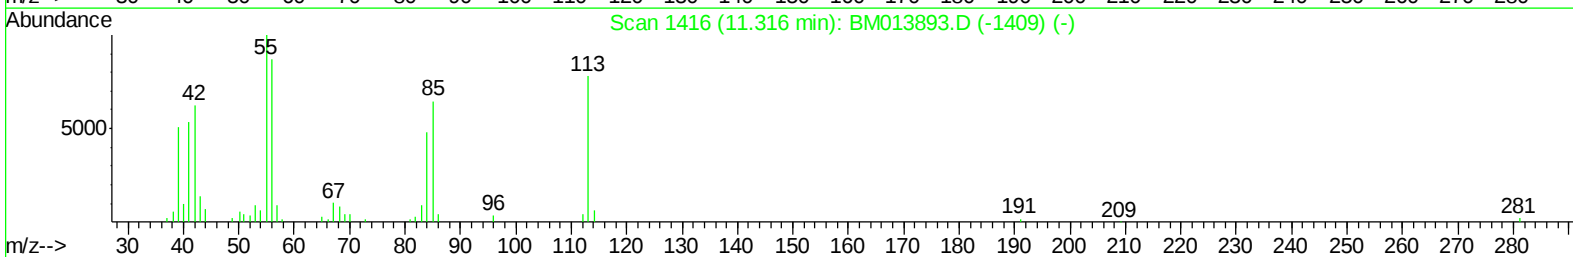
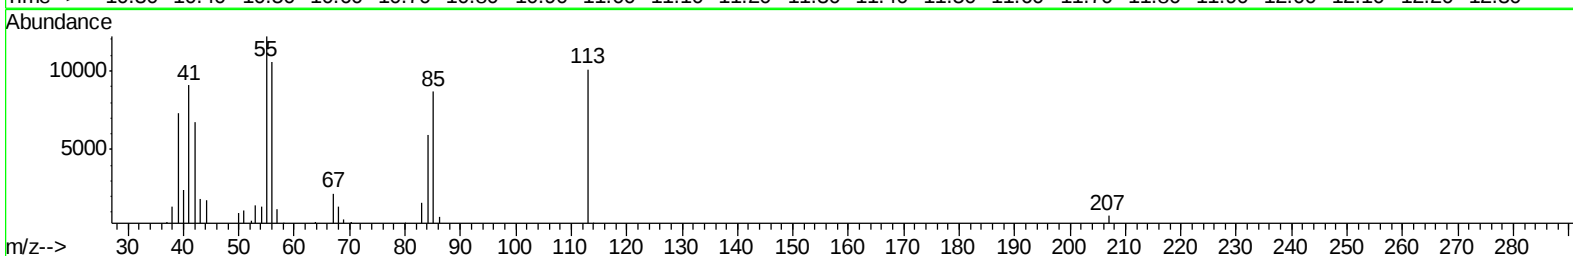


Data File : BM013920.D
Acq On : 28 Jan 2018 13:52
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 29 02:13:45 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jan 28 02:49:11 2018
Response via : Initial Calibration

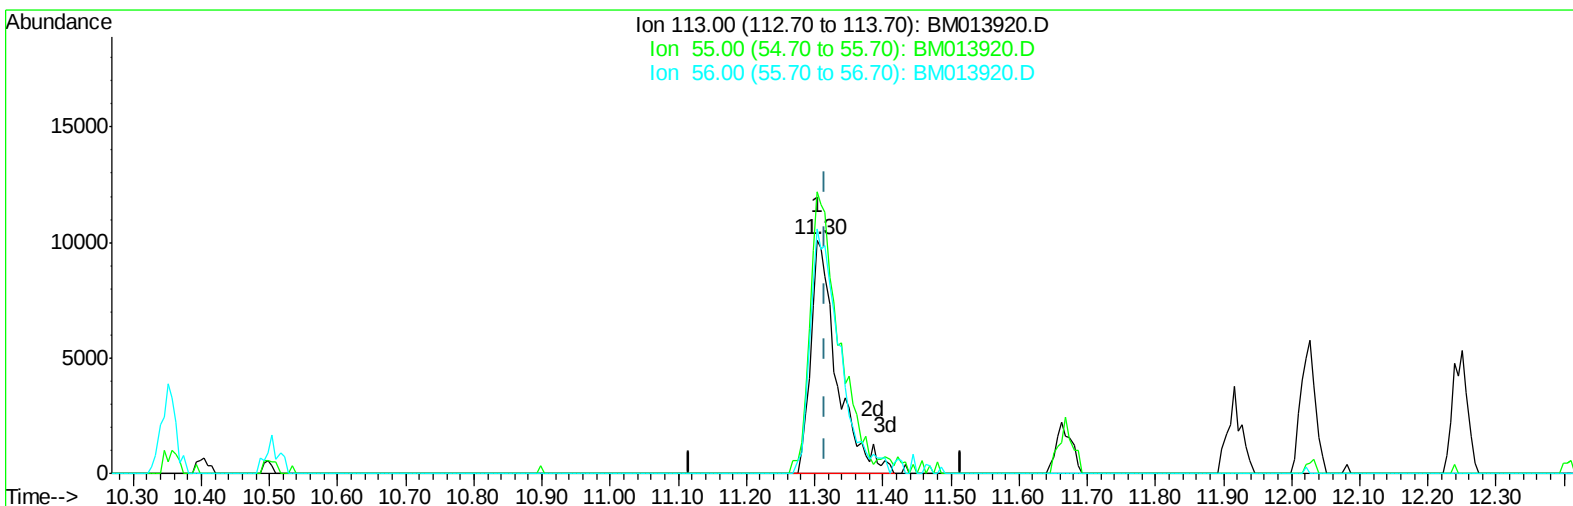

TIC: BM013920.D

(32) Caprolactam

11.304min (-0.012) 17.98ng/ul m

response 26894

Ion	Exp%	Act%
113.00	100	100
55.00	260.00	120.70#
56.00	200.00	104.76#
0.00	0.00	0.00