
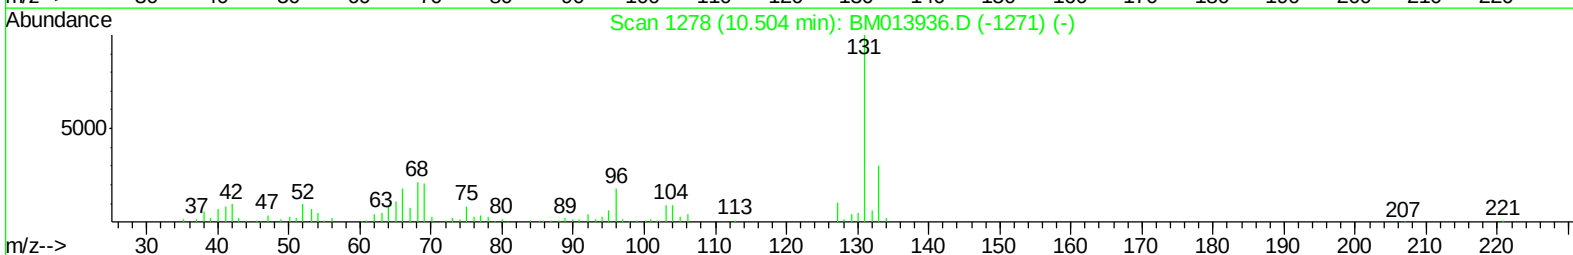
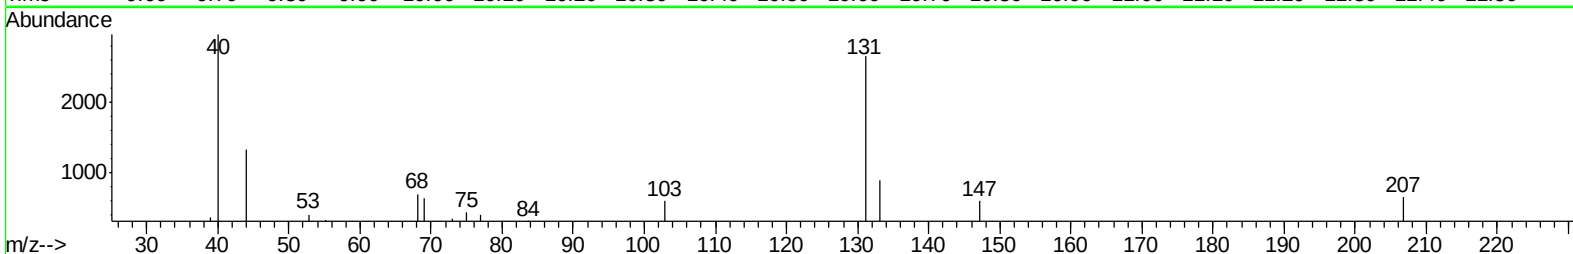


Data File : BM013943.D
Acq On : 29 Jan 2018 03:37
Operator : SJ/JU
Sample : J1233-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Jan 29 06:10:35 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 29 04:03:39 2018
Response via : Initial Calibration

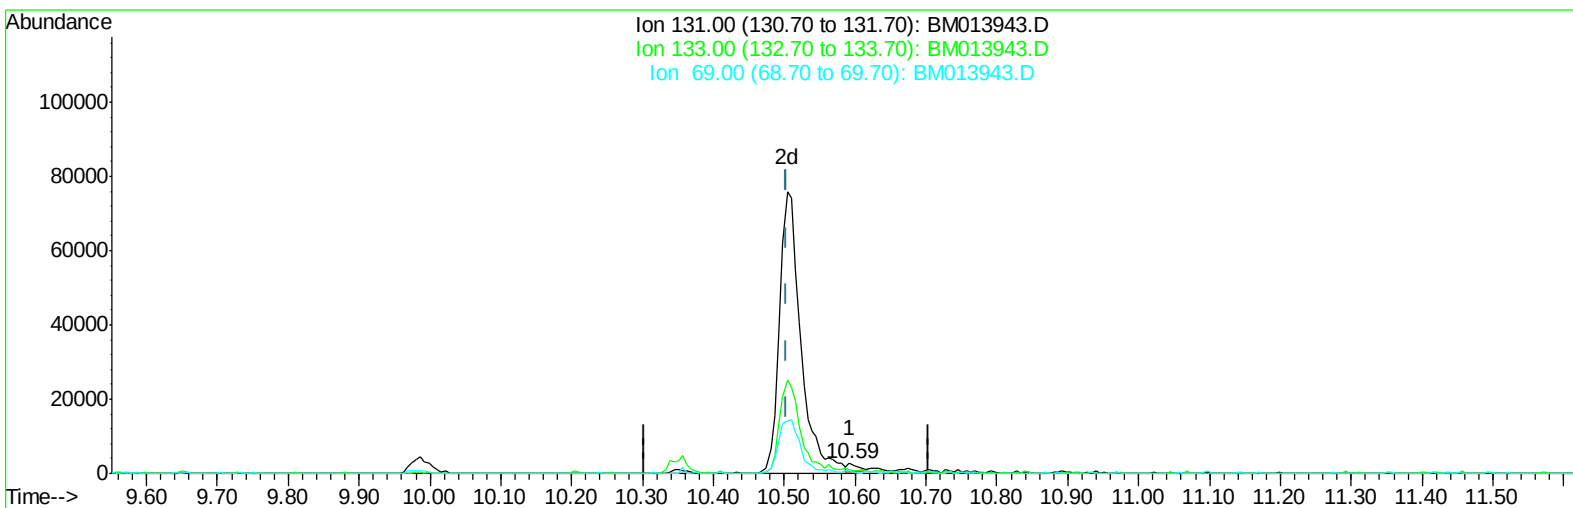

TIC: BM013943.D

(29) 4-Chloroaniline-d4 (S)
10.592min (+0.088) 0.17ng/ul
response 2023

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	33.48
69.00	24.30	24.08
0.00	0.00	0.00