
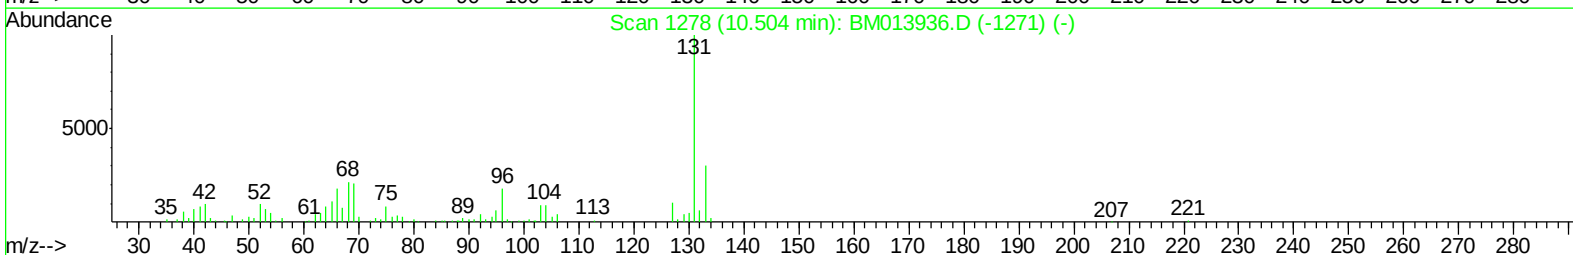
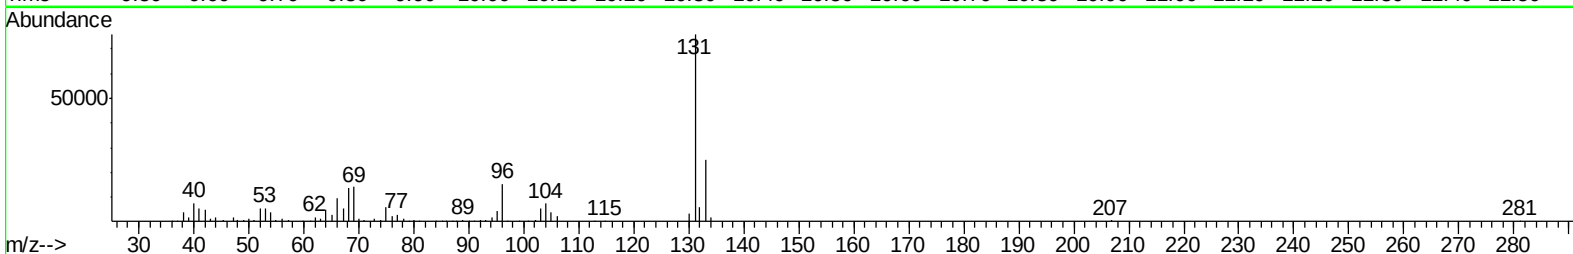


Data File : BM013943.D  
Acq On : 29 Jan 2018 03:37  
Operator : SJ/JU  
Sample : J1233-08  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Jan 29 06:10:35 2018  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM011018.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Jan 29 04:03:39 2018  
Response via : Initial Calibration

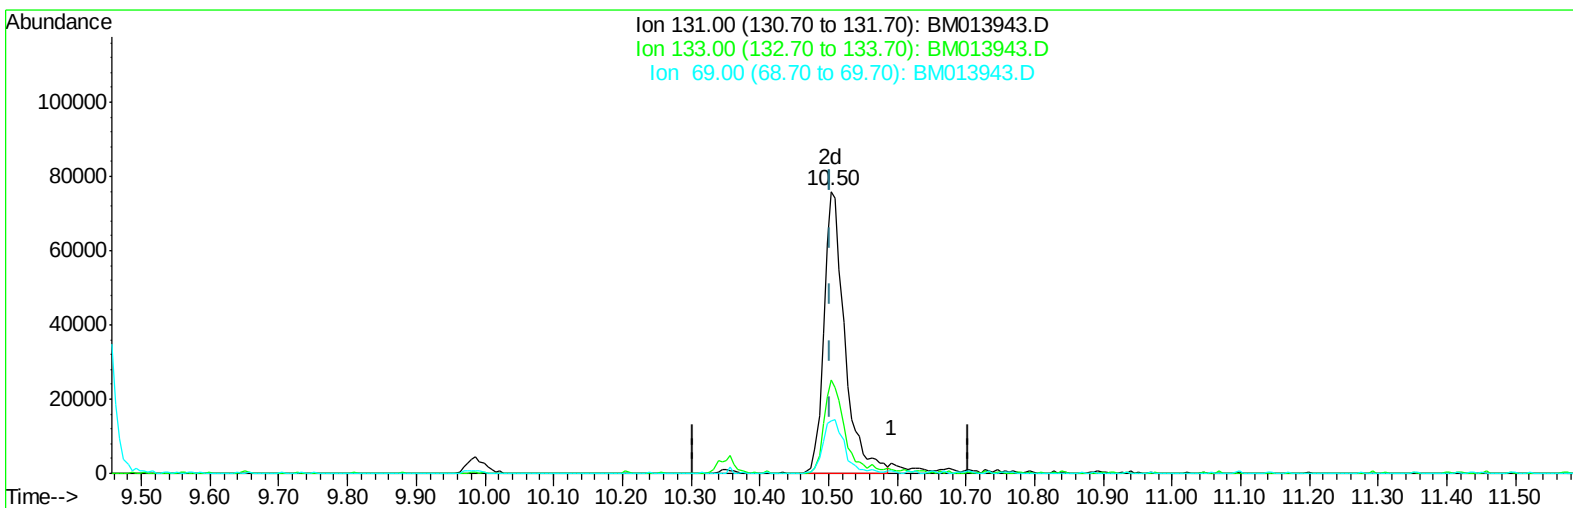

TIC: BM013943.D

(29) 4-Chloroaniline-d4 (S)

10.504min (0.000) 13.23ng/ul m

response 159887

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 131.00 | 100   | 100    |
| 133.00 | 31.40 | 33.10  |
| 69.00  | 24.30 | 18.65# |
| 0.00   | 0.00  | 0.00   |