
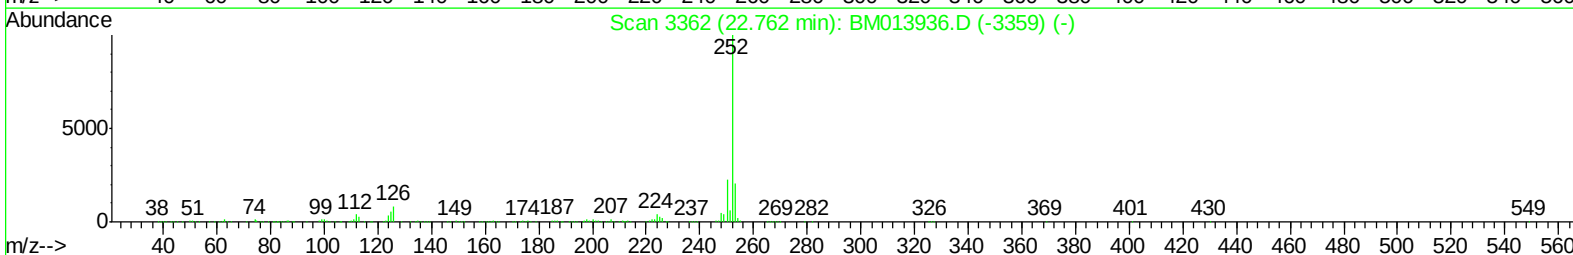
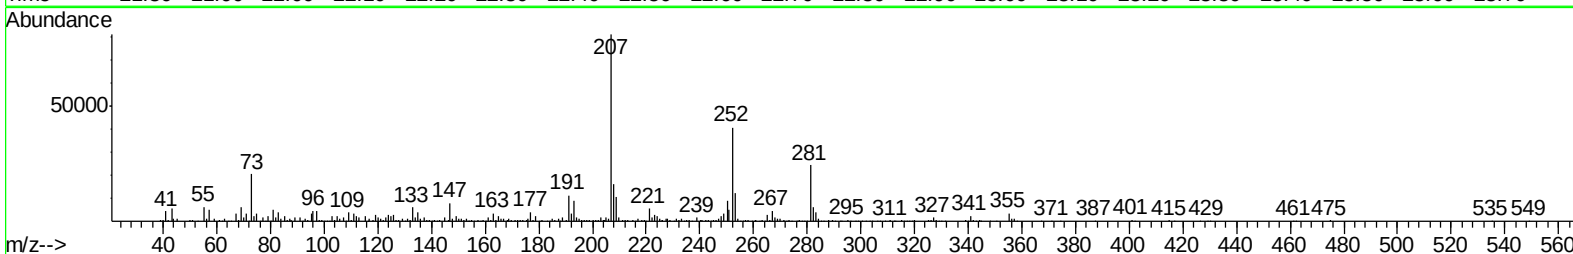


Data File : BM013945.D
Acq On : 29 Jan 2018 04:48
Operator : SJ/JU
Sample : J1243-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jan 29 07:08:02 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 29 04:03:39 2018
Response via : Initial Calibration

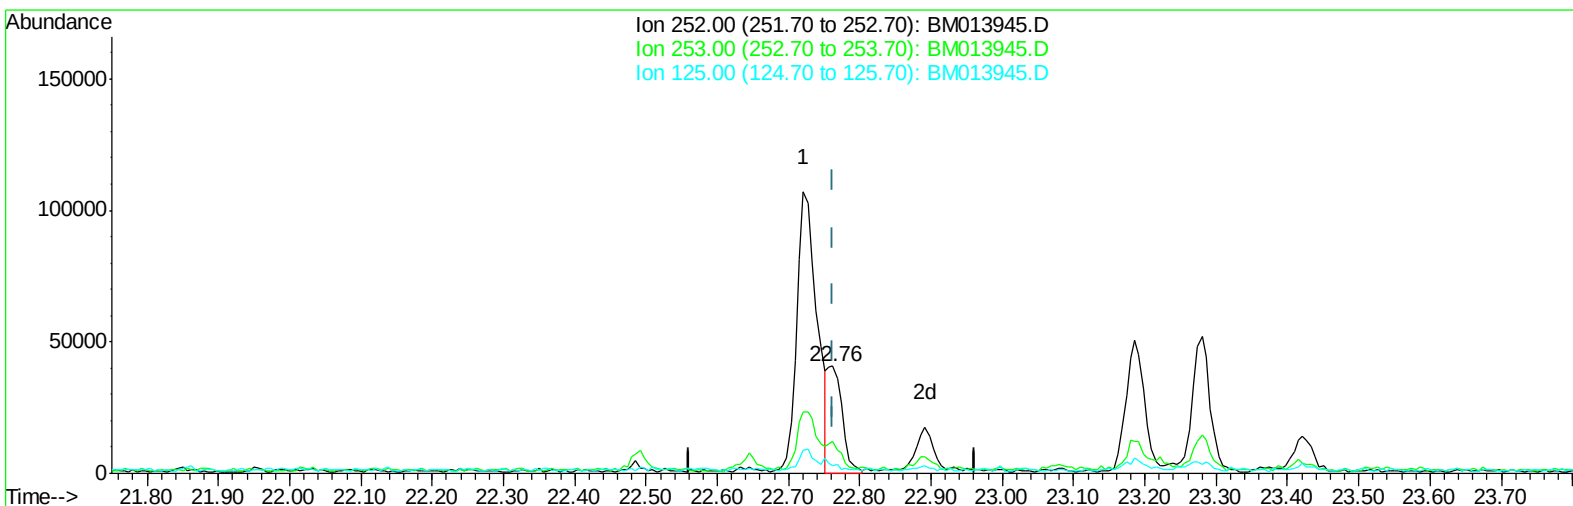

TIC: BM013945.D

(86) Benzo(k)fluoranthene

22.762min (+0.000) 1.28ng/ul m

response 59325

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	30.46#
125.00	4.30	6.66#
0.00	0.00	0.00