
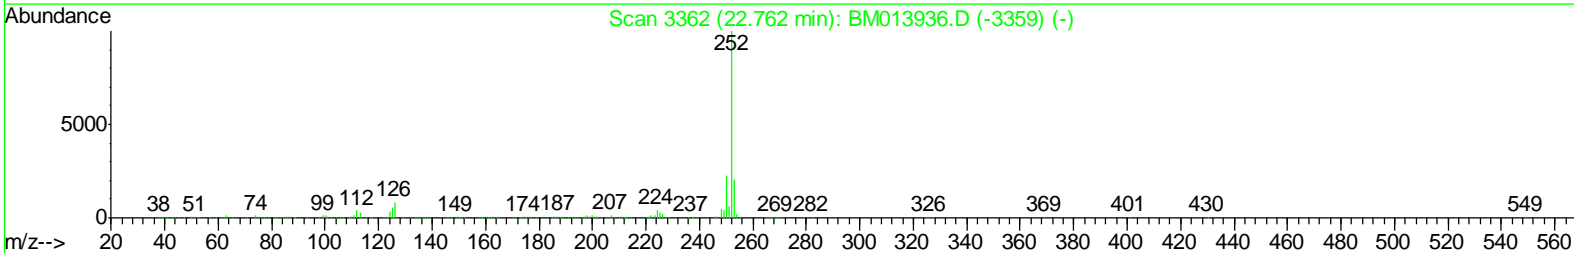
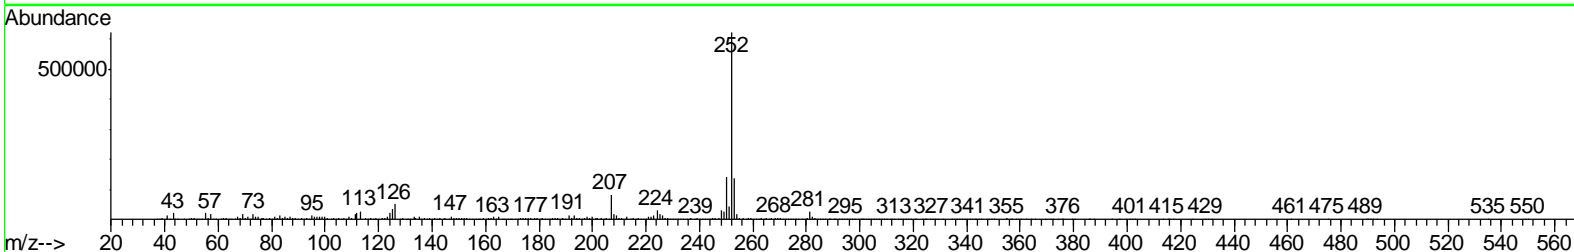


Data File : BM013947.D
Acq On : 29 Jan 2018 06:00
Operator : SJ/JU
Sample : J1243-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 29 07:14:37 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 29 04:03:39 2018
Response via : Initial Calibration

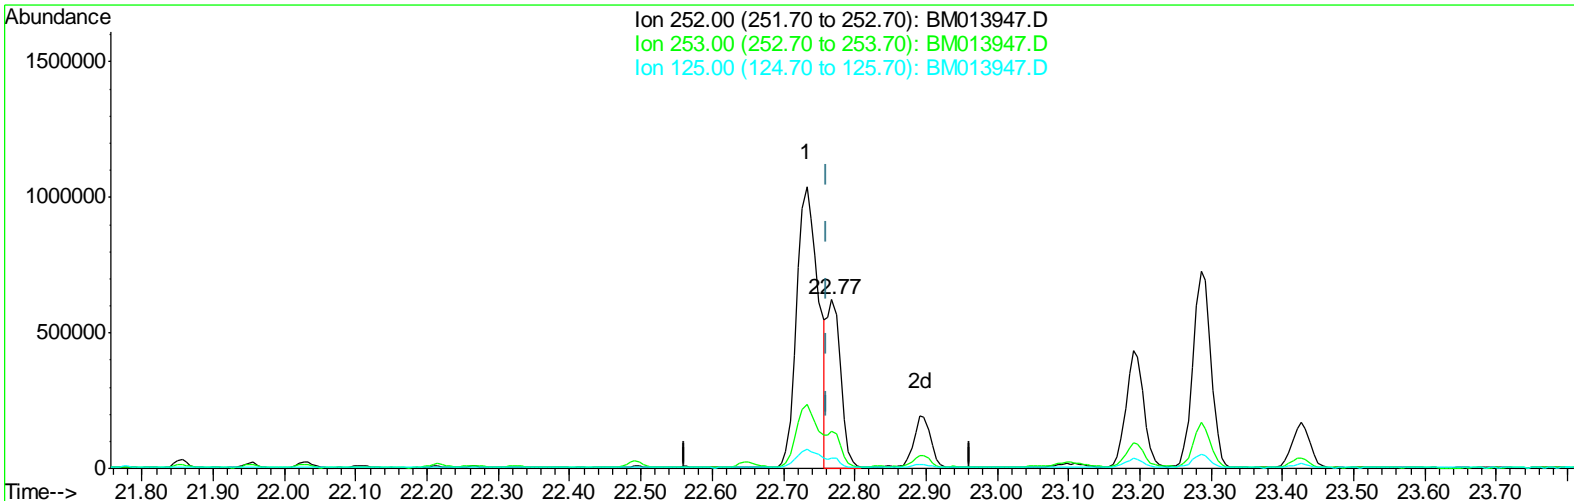

TIC: BM013947.D

(86) Benzo(k)fluoranthene
22.768min (+0.006) 16.45ng/ul m
response 849437

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.25
125.00	4.30	5.81#
0.00	0.00	0.00