

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012818\
 Data File : BM013924.D
 Acq On : 28 Jan 2018 16:16
 Operator : SJ/JU
 Sample : J1282-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6B94

Quant Time: Feb 10 00:27:46 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 29 02:34:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	139825	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	541795	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	299446	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	651199	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	720586	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	771119	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	14149	4.00	ng/uL	0.00
5) Phenol-d5	6.77	99	245320	22.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	158454	24.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	210911	24.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	201061	24.37	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	111164	26.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	117902	26.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	213829	24.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	251243	33.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	666021	26.99	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	831631	26.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	60107	14.99	ng/ul	0.00
57) Fluorene-d10	15.23	176	561909	25.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	72585	18.52	ng/ul	0.00
70) Anthracene-d10	17.09	188	844231	26.62	ng/ul	0.00
76) Pyrene-d10	19.39	212	969585	28.90	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	1040308	29.35	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.70	163	85433	3.521	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012818\
Data File : BM013924.D
Acq On : 28 Jan 2018 16:16
Operator : SJ/JU
Sample : J1282-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6B94

Quant Time: Feb 10 00:27:46 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 29 02:34:24 2018
Response via : Initial Calibration

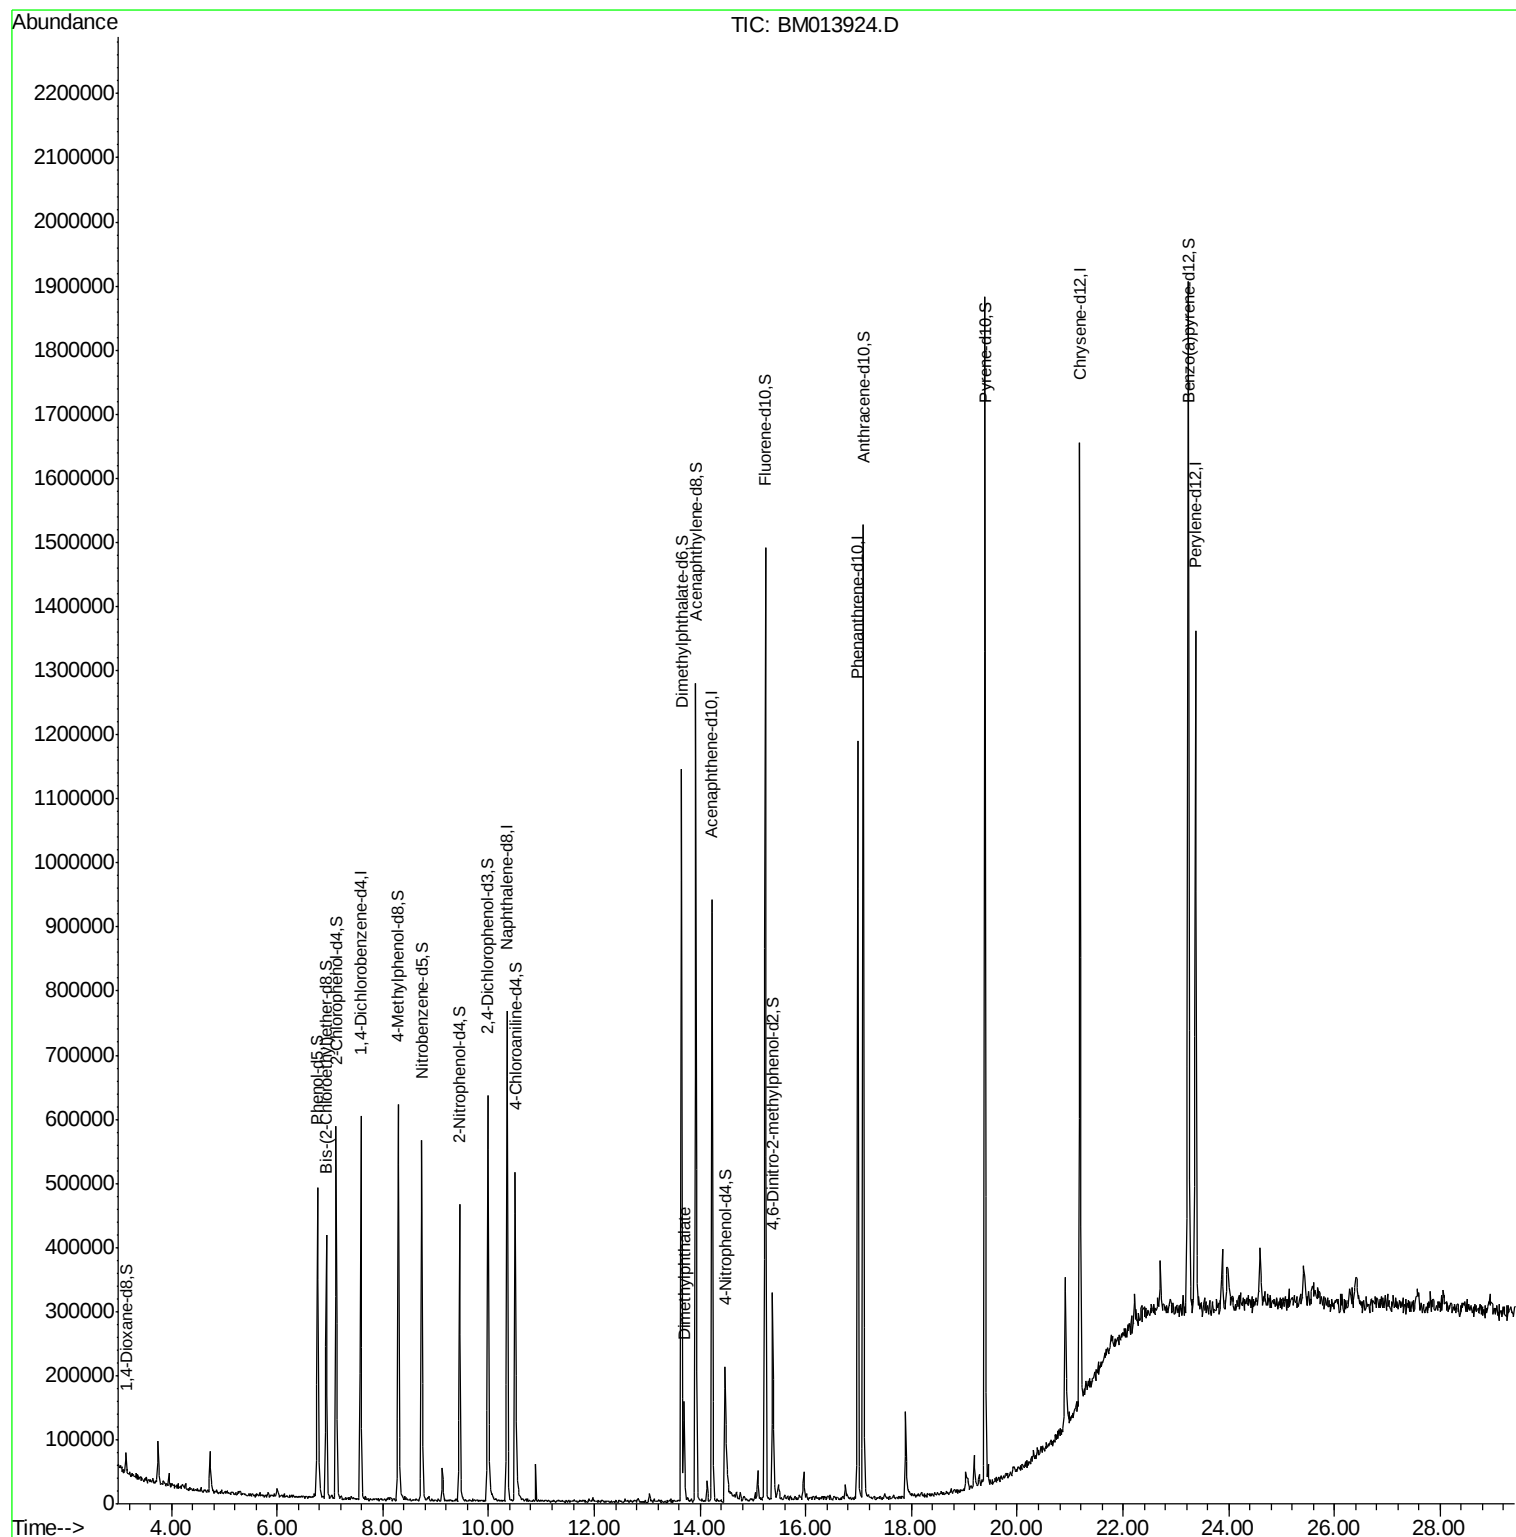

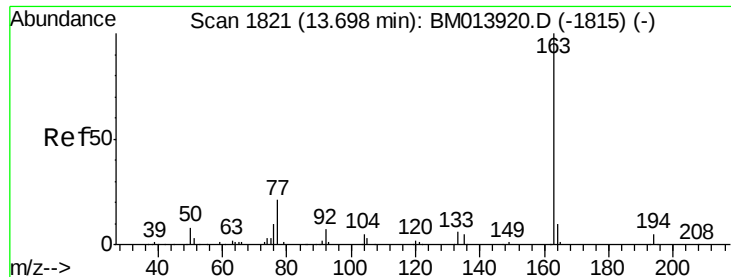

#44

Dimethylphthalate

Concen: 3.521 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. 0.00 min

Lab File: BM013924.D

Acq: 28 Jan 2018 16:16

Instrument :

BNA_M

ClientSampleId :

F6B94


Tot Ion:163 Resp: 85433

Ion Ratio Lower Upper

163 100

194 3.9 3.5 5.3

164 10.0 8.2 12.4

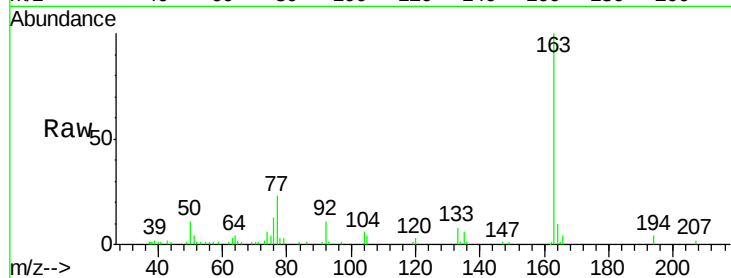

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

