

Data Path : U:\HPCHEM1\BNA M\DATA\BM012818\
 Data File : BM013931.D
 Acq On : 28 Jan 2018 20:27
 Operator : SJ/JU
 Sample : J1295-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6C16

Quant Time: Jan 29 03:09:29 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 29 02:34:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	113067	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	468605	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	303986	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	755743	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	759308	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	663240	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	14496	5.07	ng/uL	0.00
5) Phenol-d5	6.76	99	268575	30.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	175842	33.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	233271	32.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	242520	36.35	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	120294	33.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	135403	35.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	250638	33.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	288269	44.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	856502	34.19	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1067949	33.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	91417	22.45	ng/ul	0.00
57) Fluorene-d10	15.23	176	775895	35.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	107284	23.58	ng/ul	0.00
70) Anthracene-d10	17.09	188	1254077	34.07	ng/ul	0.00
76) Pyrene-d10	19.39	212	1467104	41.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	1125887	36.93	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	6.79	94	17589	2.020	ng/ul	92
44) Dimethylphthalate	13.70	163	136492	5.541	ng/ul	98
68) Pentachlorophenol	16.65	266	9543	1.869	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA M\DATA\BM012818\
Data File : BM013931.D
Acq On : 28 Jan 2018 20:27
Operator : SJ/JU
Sample : J1295-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6C16

Quant Time: Jan 29 03:09:29 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 29 02:34:24 2018
Response via : Initial Calibration

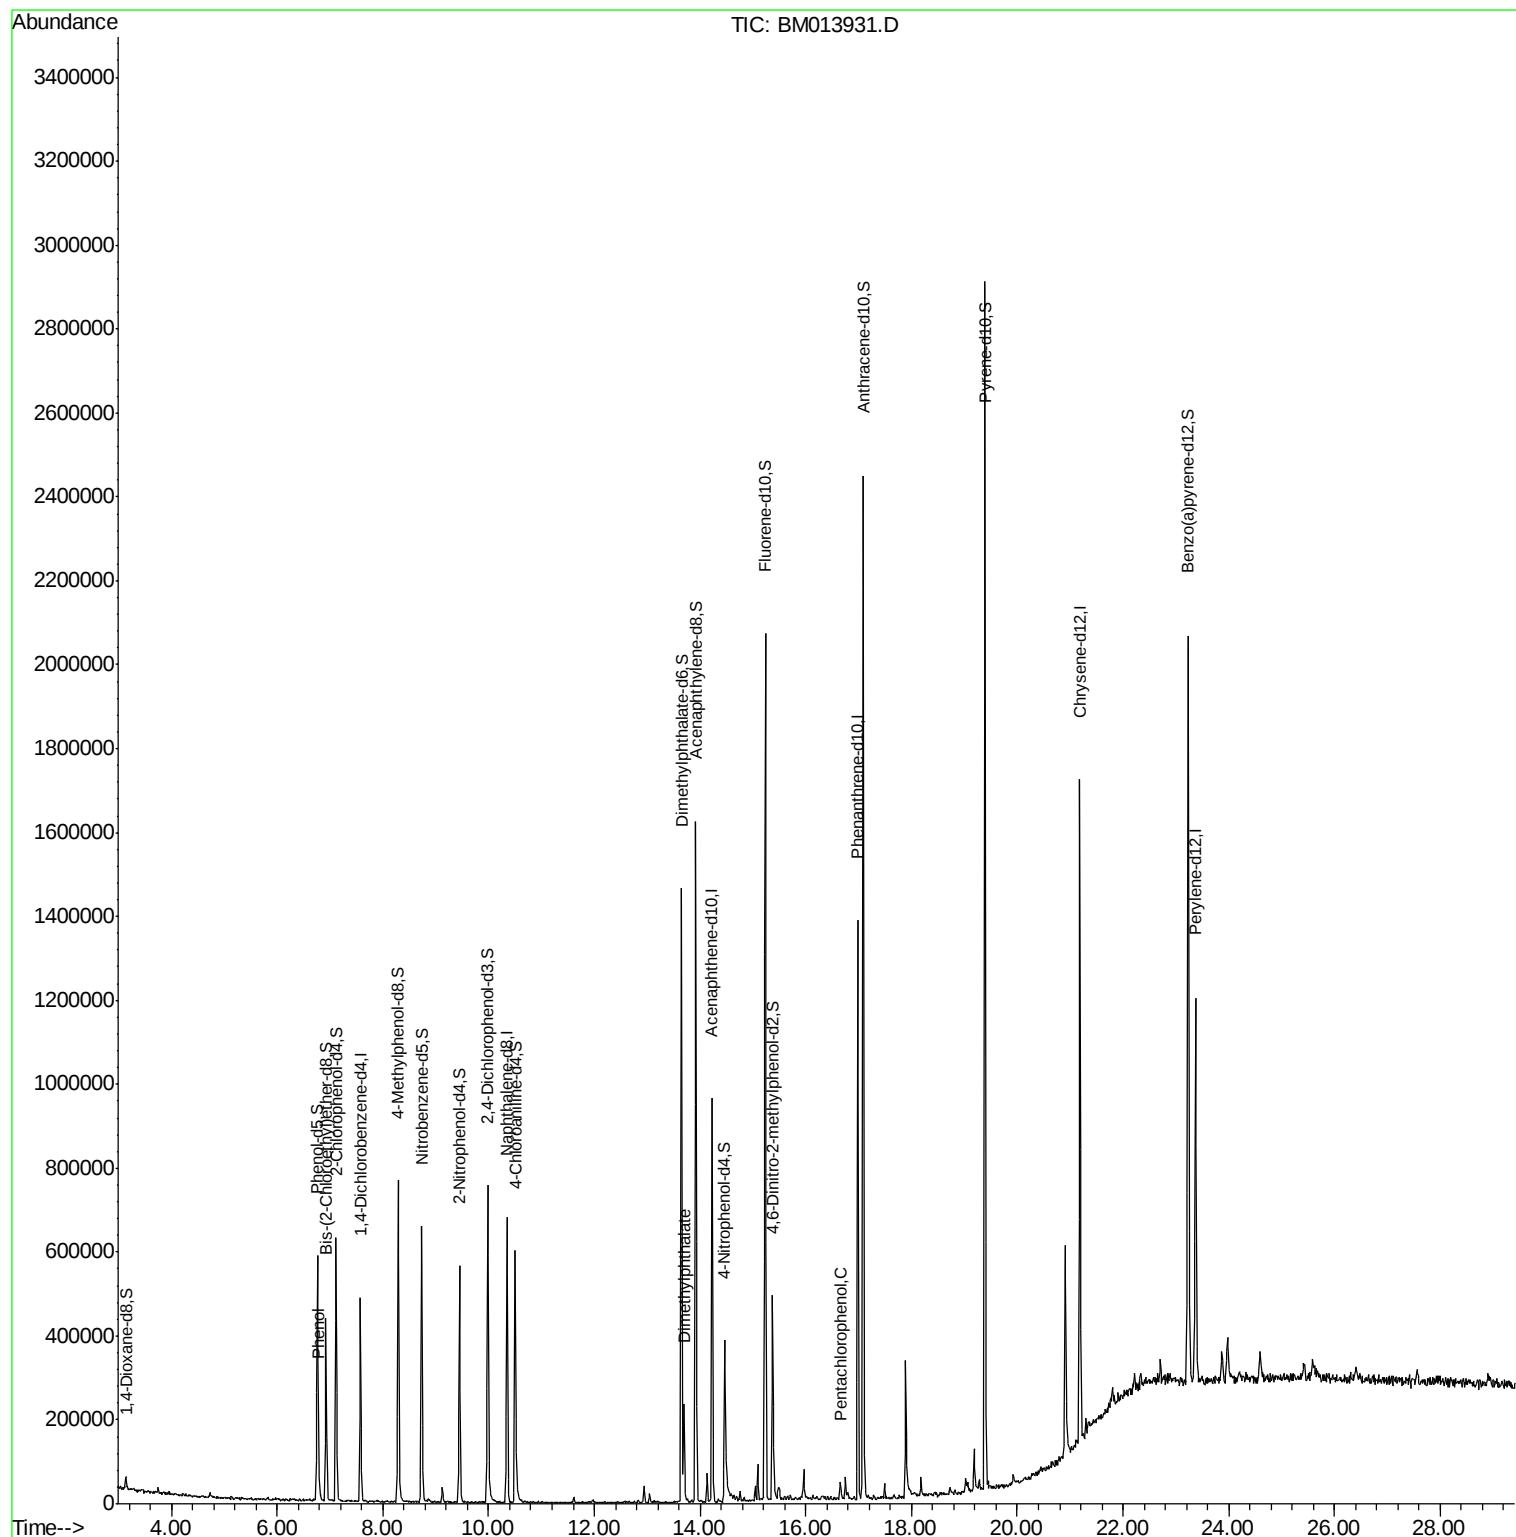

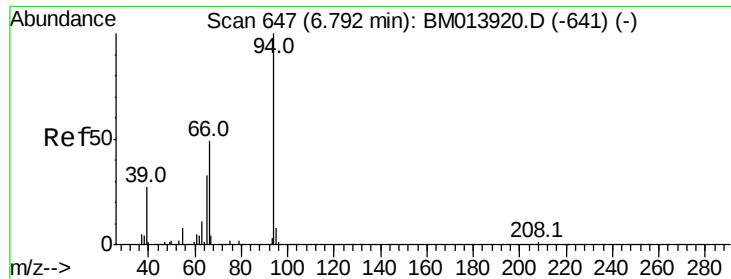

#6

Phenol

Concen: 2.020 ng/ul

RT: 6.79 min Scan# 646

Delta R.T. -0.01 min

Lab File: BM013931.D

Acq: 28 Jan 2018 20:27

Instrument :

BNA_M

ClientSampleId :

F6C16





Tot Ion: 94 Resp: 17589

Ion Ratio Lower Upper

94 100

65 37.3 28.2 42.4

66 67.5 47.2 70.8

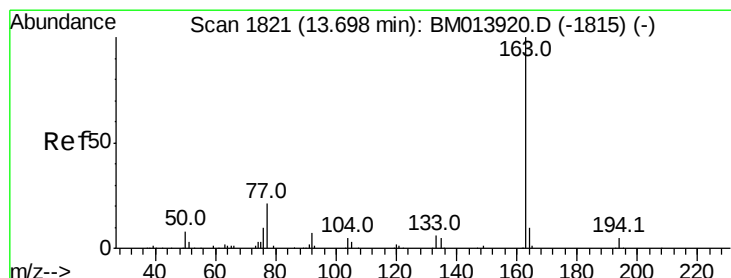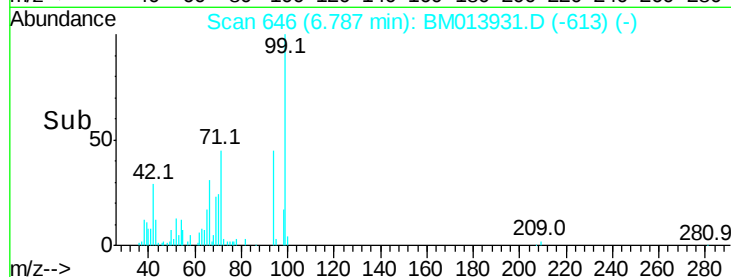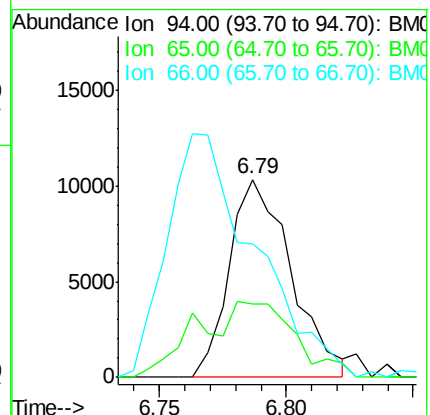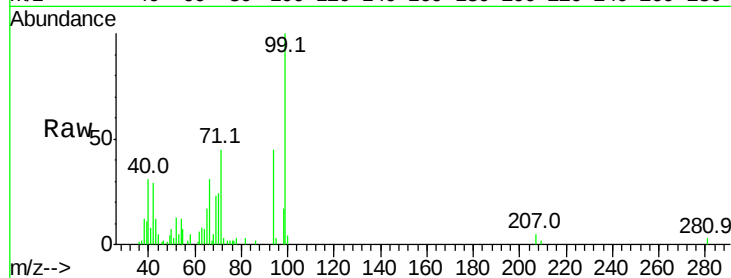

#44

Dimethylphthalate

Concen: 5.541 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. 0.00 min

Lab File: BM013931.D

Acq: 28 Jan 2018 20:27




Tgt Ion: 163 Resp: 136492


Ion Ratio Lower Upper

163 100

194 5.0 3.5 5.3

164 9.6 8.2 12.4

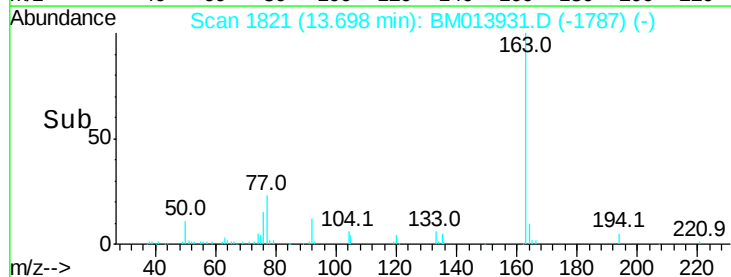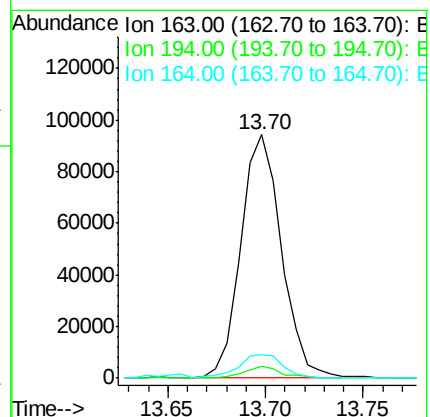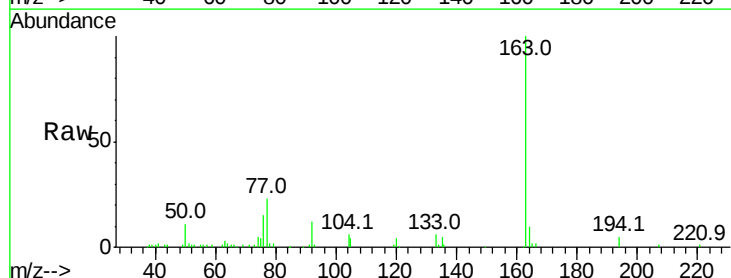

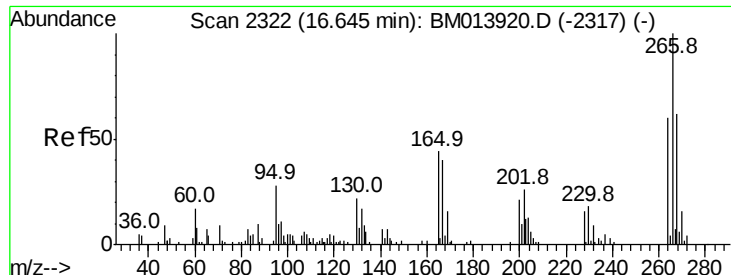

#68

Pentachlorophenol

Concen: 1.869 ng/ul

RT: 16.65 min Scan# 2323

Delta R.T. 0.01 min

Lab File: BM013931.D

Acq: 28 Jan 2018 20:27

Instrument :

BNA_M

ClientSampleId :

F6C16


Tot Ion:266 Resp: 9543

Ion Ratio Lower Upper

266 100

264 58.7 49.3 73.9

268 52.3 52.6 78.8#

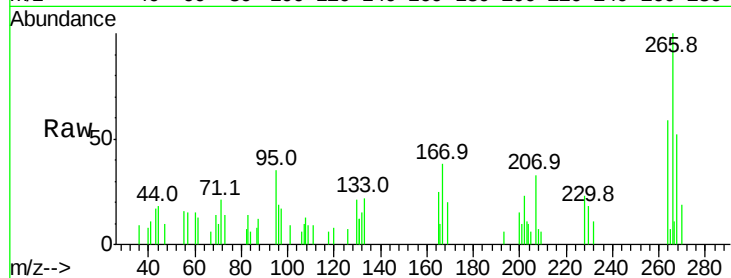

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

