
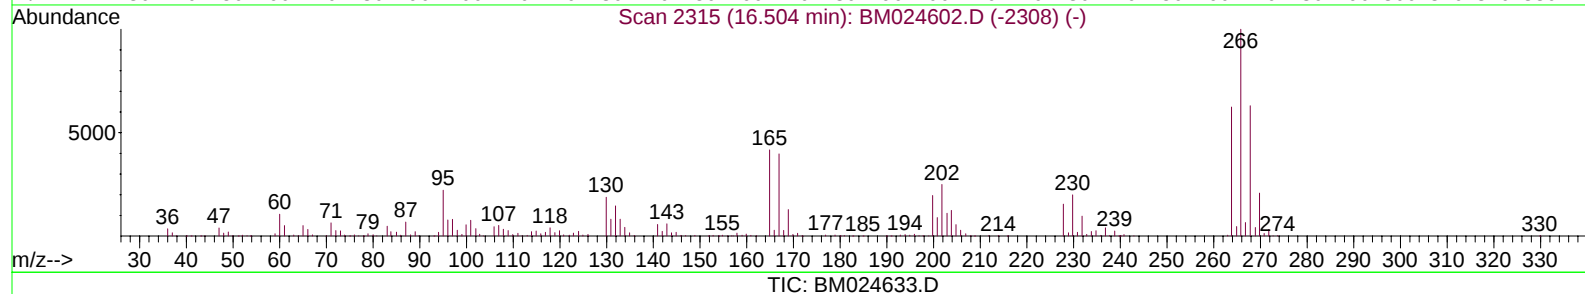
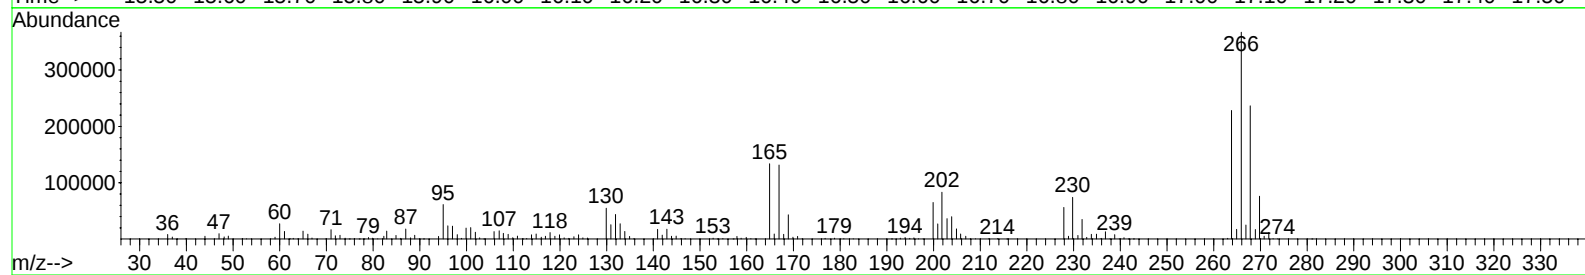


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012820\
Data File : BM024633.D
Acq On : 28 Jan 2020 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 17:57:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 23 14:57:07 2020
Response via : Initial Calibration

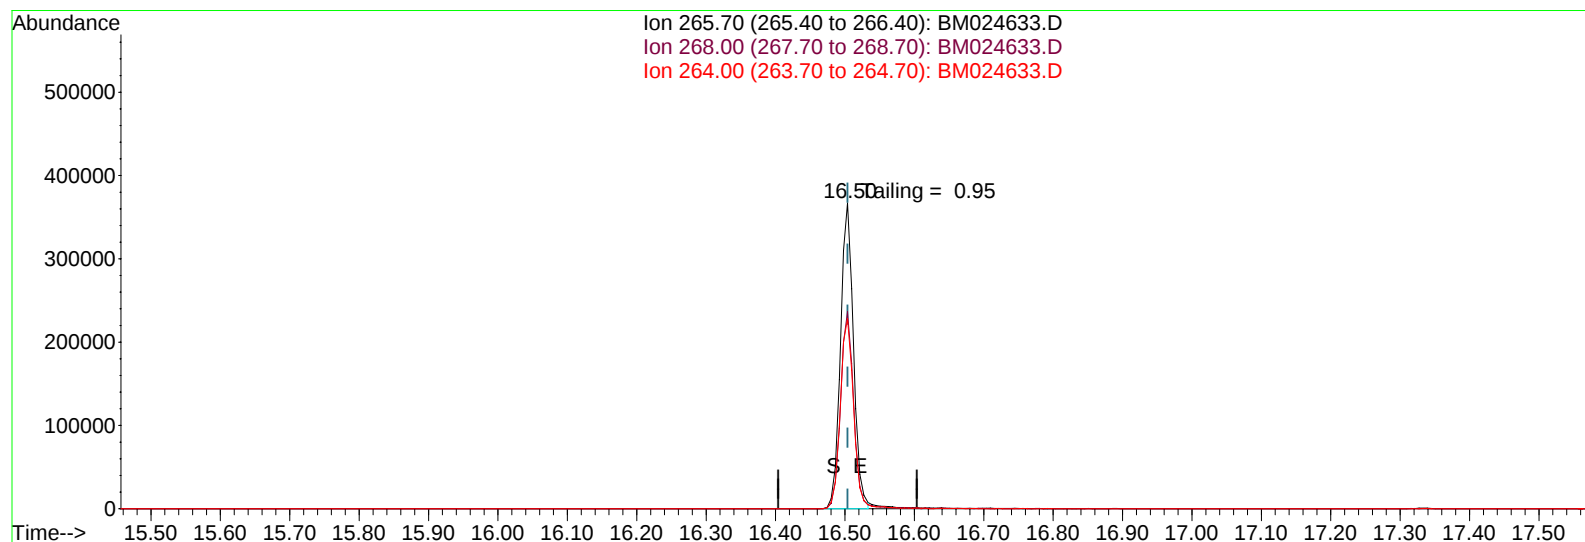

(70) Pentachlorophenol (C)




16.504min (+0.000) 189886.44ng

response 481974

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	64.39
264.00	62.40	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012820\
 Data File : BM024633.D
 Acq On : 28 Jan 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 17:57:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

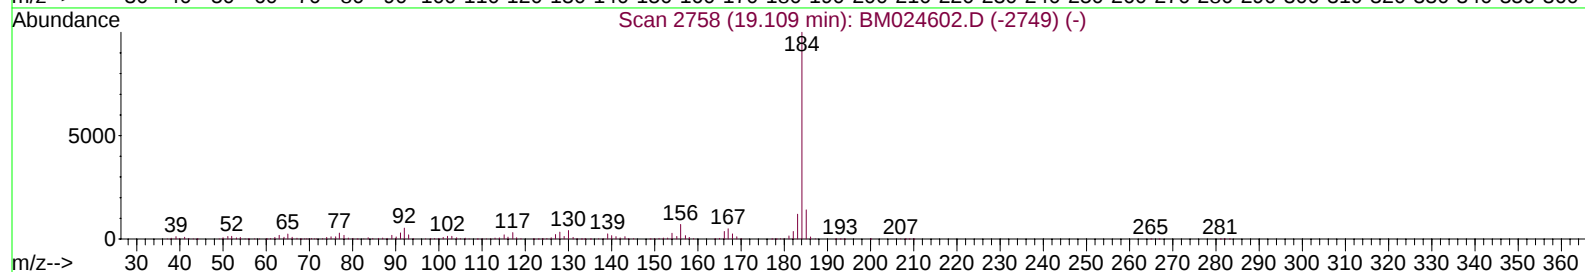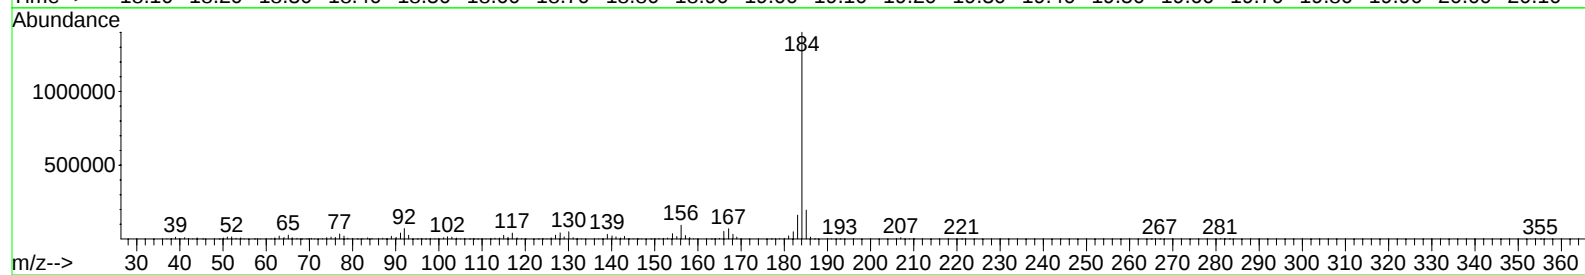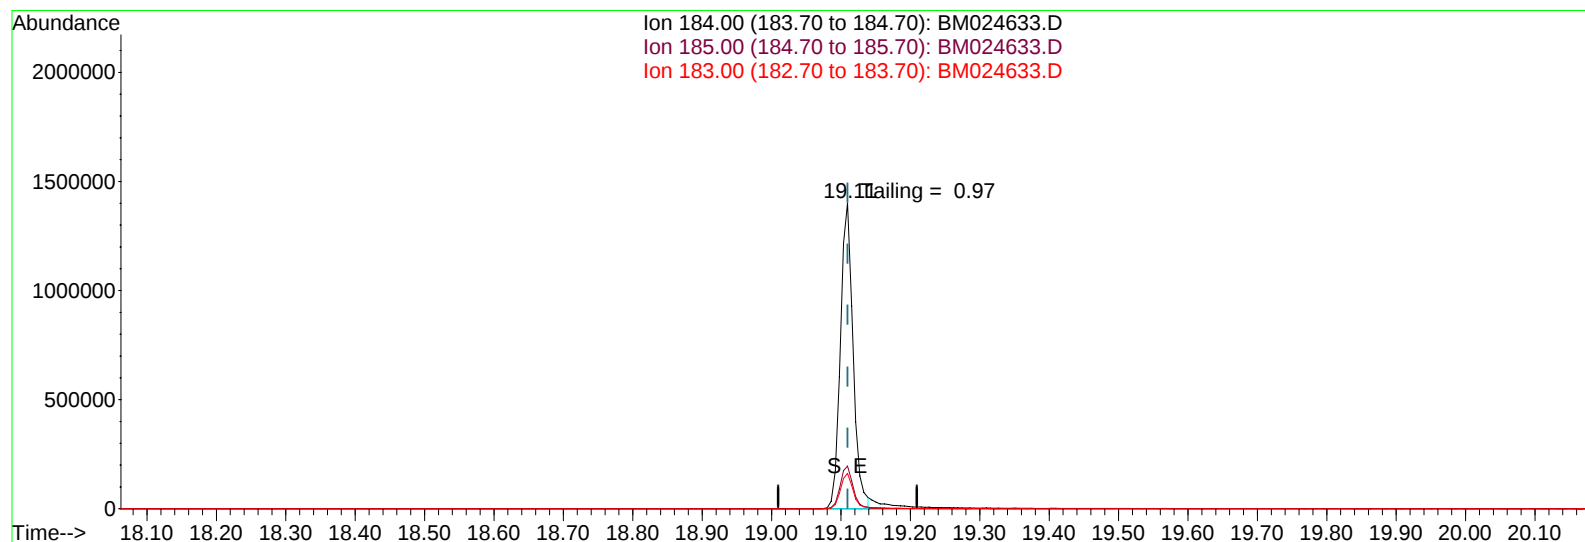

TIC: BM024633.D

(77) Benzidine

19.109min (+0.000) 15356.16ng

response 1831037

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.96
183.00	12.00	11.57
0.00	0.00	0.00