


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012821\
 Data File : BM028582.D
 Acq On : 28 Jan 2021 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 27 13:20:04 2021

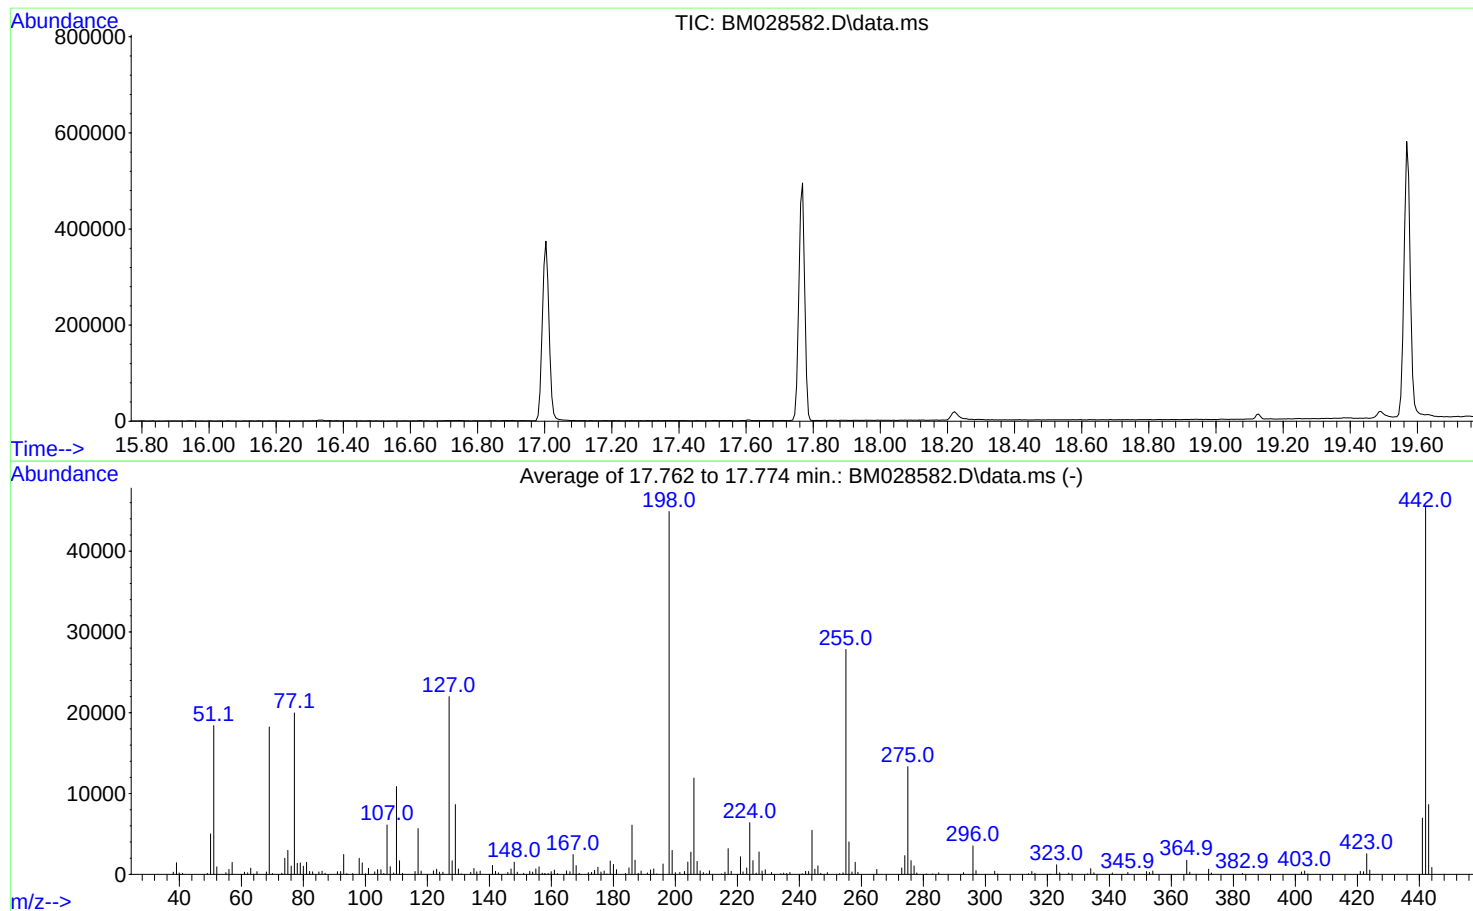

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	18408	PASS
68	69	0.00	2	1.6	288	PASS
69	198	0.00	100	40.6	18233	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	49.0	21989	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44899	PASS
199	198	5	9	6.6	2981	PASS
275	198	10	60	29.7	13324	PASS
365	198	1	100	3.9	1753	PASS
441	198	0.01	100	15.5	6969	PASS
442	442	50	100	100.0	45520	PASS
443	442	15	24	19.0	8631	PASS