

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049513.D
 Acq On : 29 Jan 2025 20:53
 Operator : RC/JU
 Sample : Q1184-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2961

Quant Time: Jan 30 07:34:33 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	200644	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	759040	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	493707	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	1015408	20.000	ng/ul	0.00
79) Chrysene-d12	21.133	240	1066966	20.000	ng/ul	0.00
88) Perylene-d12	23.909	264	1149964	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	30048	5.549	ng/uL	0.00
4) Pyridine-d5	3.516	84	131581	8.270	ng/ul	0.00
7) Phenol-d5	6.734	99	195665	12.017	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	373522	33.549	ng/ul	0.00
11) 2-Chlorophenol-d4	7.063	132	442772	35.143	ng/ul	0.01
15) 4-Methylphenol-d8	8.245	113	318955	26.738	ng/ul	0.02
21) Nitrobenzene-d5	8.657	128	215617	37.131	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	251188	39.657	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.922	165	457611	35.404	ng/ul	0.02
31) 4-Chloroaniline-d4	10.422	131	401516	24.217	ng/ul	0.00
46) Dimethylphthalate-d6	13.574	166	1434544	39.629	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	1570293	36.920	ng/ul	0.00
54) 4-Nitrophenol-d4	14.445	143	50987	8.586	ng/ul	0.06
60) Fluorene-d10	15.151	176	1254736	39.415	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.286	200	228465	35.705	ng/ul	0.00
73) Anthracene-d10	17.004	188	2143564	42.274	ng/ul	0.00
81) Pyrene-d10	19.309	212	2711191	43.467	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	2750555	44.846	ng/ul	0.00


Target Compounds					Qvalue
35) 4-Chloro-3-methylphenol	11.645	107	750184	66.825 ng/ul#	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049513.D
Acq On : 29 Jan 2025 20:53
Operator : RC/JU
Sample : Q1184-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2961

Quant Time: Jan 30 07:34:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

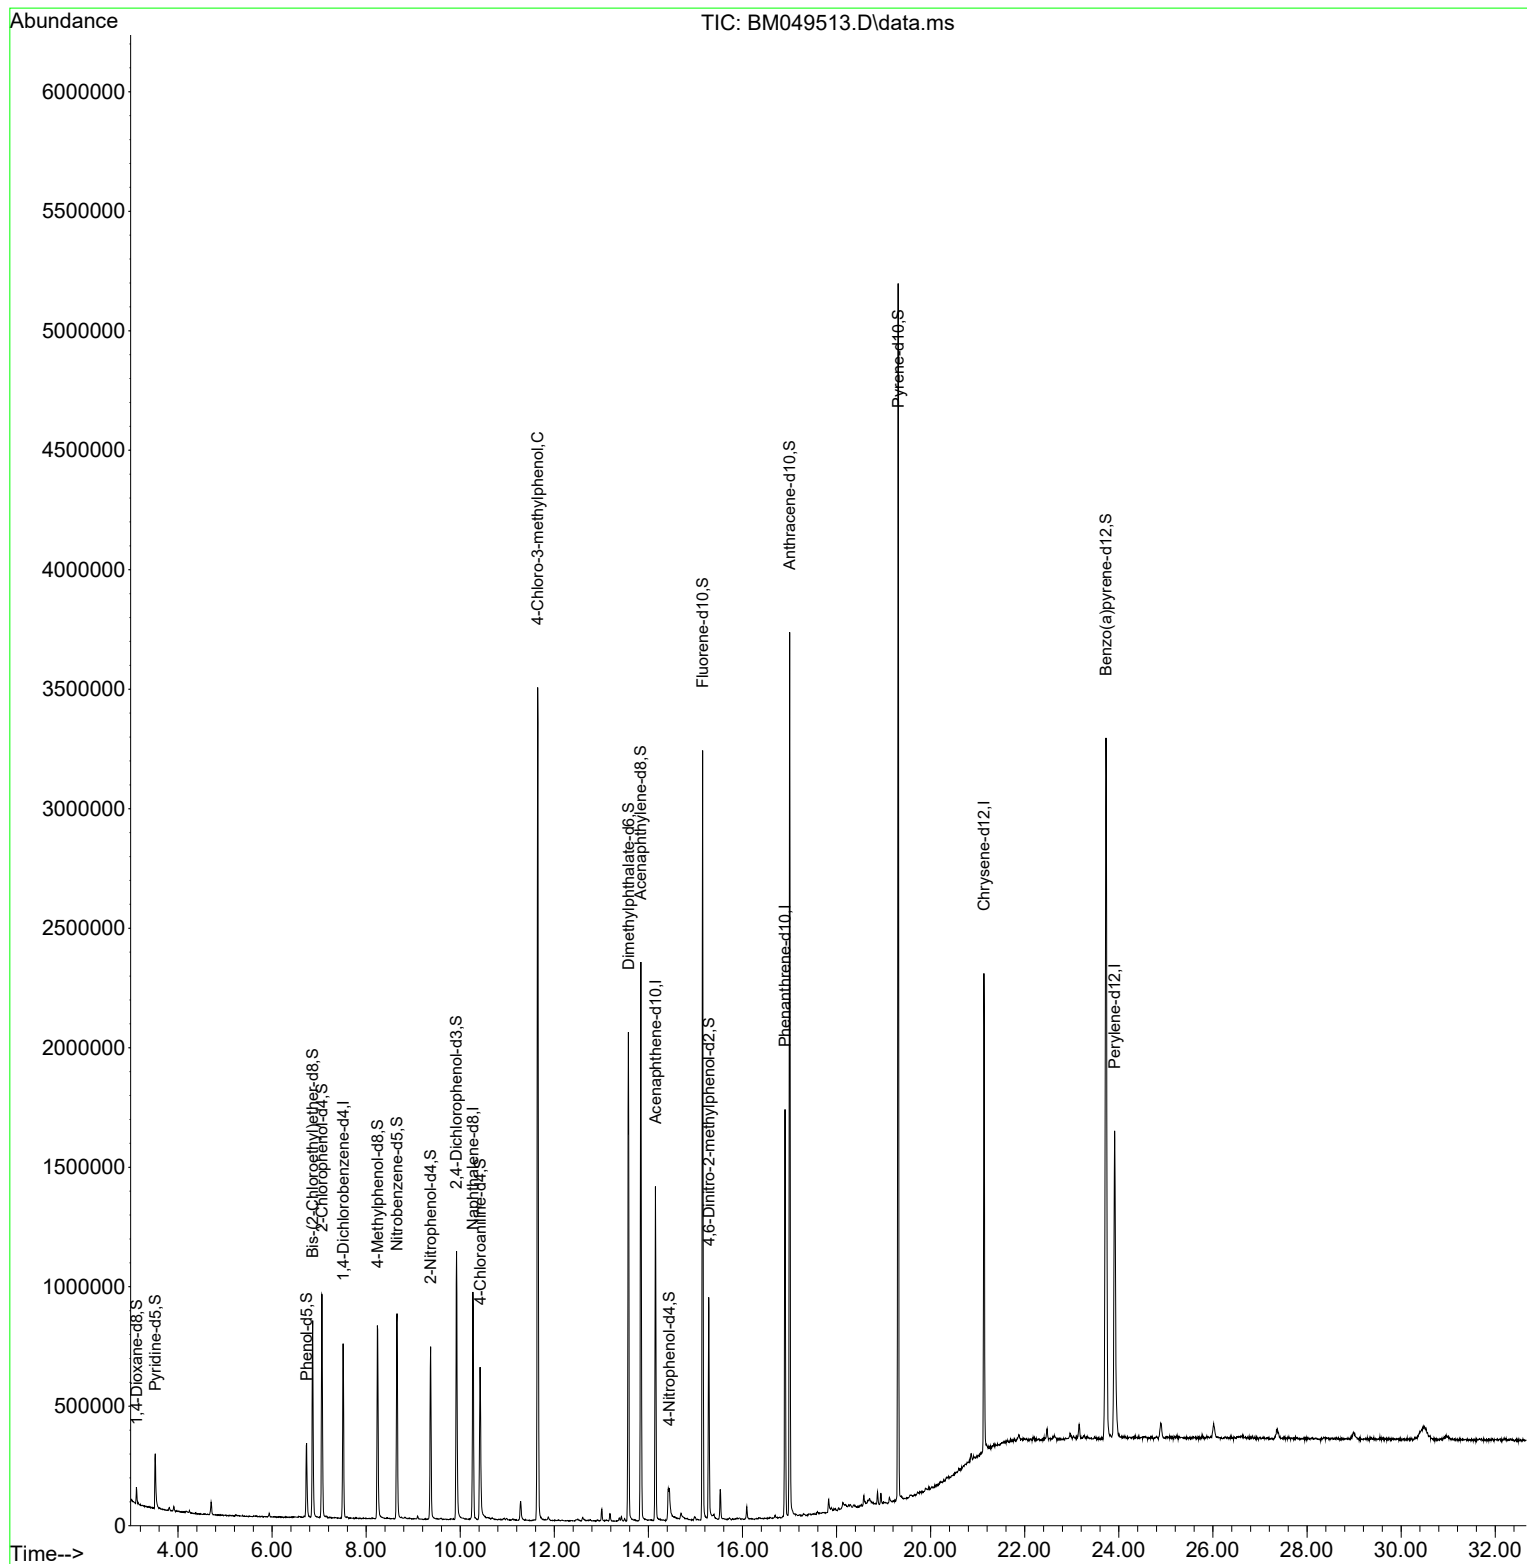

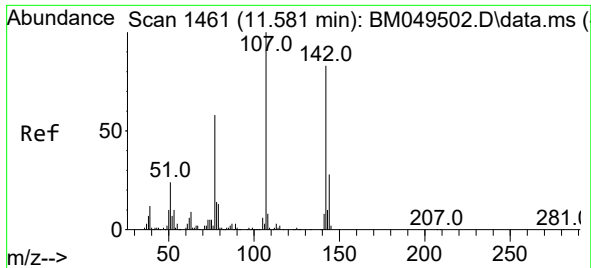

#35
 4-Chloro-3-methylphenol
 Concen: 66.825 ng/ul
 RT: 11.645 min Scan# 14
 Delta R.T. 0.064 min
 Lab File: BM049513.D
 Acq: 29 Jan 2025 20:53

Instrument :
 BNA_M
 ClientSampleId :
 E2961

Tgt Ion:107 Resp: 750184
 Ion Ratio Lower Upper
 107 100
 144 0.0 22.6 34.0#
 142 0.0 67.5 101.3#

